

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029632.D
 Acq On : 10 Feb 2024 04:57
 Operator : MA/JU
 Sample : P1398-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	46	rBV	56290	70214	1.67%	0.156%
2	3.746	109	112	126	rBV	139814	250962	5.96%	0.559%
3	4.064	163	166	172	rVB	28498	37287	0.89%	0.083%
4	5.017	324	328	334	rVB7	3983	6026	0.14%	0.013%
5	5.528	409	415	422	rBV8	7544	18693	0.44%	0.042%
6	5.887	472	476	478	rVB4	4877	5401	0.13%	0.012%
7	7.046	666	673	681	rBV	239571	372123	8.84%	0.829%
8	7.222	697	703	721	rVB	933883	1488554	35.37%	3.315%
9	7.411	727	735	744	rBV	857419	1384345	32.90%	3.082%
10	7.499	746	750	752	rVV5	2855	4621	0.11%	0.010%
11	7.881	808	815	825	rVB	891106	1383268	32.87%	3.080%
12	8.587	928	935	950	rBV	623117	1017185	24.17%	2.265%
13	9.046	1006	1013	1028	rBV	1028989	1669183	39.67%	3.717%
14	9.216	1037	1042	1046	rBV7	4111	6834	0.16%	0.015%
15	9.763	1128	1135	1145	rBV	691037	1171549	27.84%	2.609%
16	10.299	1217	1226	1239	rBV	1063965	1749381	41.57%	3.895%
17	10.681	1282	1291	1300	rVB	1096075	1834514	43.60%	4.085%
18	10.822	1307	1315	1330	rBV	852041	1532925	36.43%	3.413%
19	11.504	1429	1431	1438	rVB5	4012	6034	0.14%	0.013%
20	12.275	1557	1562	1567	rBV2	16039	29633	0.70%	0.066%
21	13.428	1752	1758	1762	rBV3	14453	23593	0.56%	0.053%
22	13.946	1836	1846	1857	rBV	1795296	2482938	59.00%	5.529%
23	14.216	1885	1892	1907	rBV	2106160	3042644	72.30%	6.775%
24	14.522	1937	1944	1953	rBV	1344174	1948825	46.31%	4.339%
25	14.722	1972	1978	1991	rBV	82422	173092	4.11%	0.385%
26	14.940	2012	2015	2018	rBV5	4486	6401	0.15%	0.014%
27	15.381	2085	2090	2095	rVB8	7054	10884	0.26%	0.024%
28	15.516	2106	2113	2127	rBV	2435039	3586926	85.24%	7.987%
29	15.640	2127	2134	2148	rVV	654316	879786	20.91%	1.959%
30	15.757	2150	2154	2159	rBV4	10922	18793	0.45%	0.042%
31	16.251	2233	2238	2239	rBV4	14424	17781	0.42%	0.040%
32	16.275	2239	2242	2245	rVV4	14956	22115	0.53%	0.049%
33	16.304	2245	2247	2251	rVB4	8311	9676	0.23%	0.022%
34	16.598	2292	2297	2299	rBV5	2844	5015	0.12%	0.011%
35	16.687	2307	2312	2319	rBV6	10136	16463	0.39%	0.037%
36	16.781	2324	2328	2333	rVV5	4491	7503	0.18%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029632.D
 Acq On : 10 Feb 2024 04:57
 Operator : MA/JU
 Sample : P1398-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAH0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	16.957	2353	2358	2362	rBV6	3457	5798	0.14%	0.013%
38	17.045	2369	2373	2378	rBV4	18465	26051	0.62%	0.058%
39	17.092	2378	2381	2386	rVB5	11076	15458	0.37%	0.034%
40	17.275	2404	2412	2419	rBV	1413251	1985896	47.19%	4.422%
41	17.375	2422	2429	2440	rBV2	2569753	3702272	87.98%	8.244%
42	17.575	2460	2463	2469	rVB6	6973	12848	0.31%	0.029%
43	17.786	2495	2499	2504	rBV	20763	26469	0.63%	0.059%
44	18.051	2541	2544	2549	rBV6	7723	12538	0.30%	0.028%
45	18.181	2561	2566	2574	rBV	111017	159149	3.78%	0.354%
46	18.257	2577	2579	2583	rVB5	3012	4351	0.10%	0.010%
47	18.486	2615	2618	2622	rBV	21923	22305	0.53%	0.050%
48	18.622	2638	2641	2644	rBV5	3480	4777	0.11%	0.011%
49	18.704	2654	2655	2658	rBV3	4607	4241	0.10%	0.009%
50	18.898	2686	2688	2694	rVB6	3419	4963	0.12%	0.011%
51	19.122	2722	2726	2731	rBV	20877	25548	0.61%	0.057%
52	19.239	2741	2746	2751	rBV3	28126	43806	1.04%	0.098%
53	19.304	2753	2757	2762	rBV	23879	39337	0.93%	0.088%
54	19.469	2781	2785	2791	rBV2	45553	57263	1.36%	0.128%
55	19.622	2810	2811	2814	rBV3	6102	6282	0.15%	0.014%
56	19.675	2814	2820	2828	rVV	2883167	4044074	96.10%	9.005%
57	20.239	2913	2916	2919	rBV3	13426	16206	0.39%	0.036%
58	21.204	3076	3080	3085	rBV5	50066	74921	1.78%	0.167%
59	21.475	3120	3126	3139	rBV	1387342	1907462	45.33%	4.247%
60	22.751	3340	3343	3349	rVB	66254	88566	2.10%	0.197%
61	23.698	3496	3504	3517	rBV2	2094266	4208073	100.00%	9.370%
62	23.845	3523	3529	3546	rVB	1044183	2120468	50.39%	4.722%




Sum of corrected areas: 44910289

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029632.D
Acq On : 10 Feb 2024 04:57
Operator : MA/JU
Sample : P1398-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

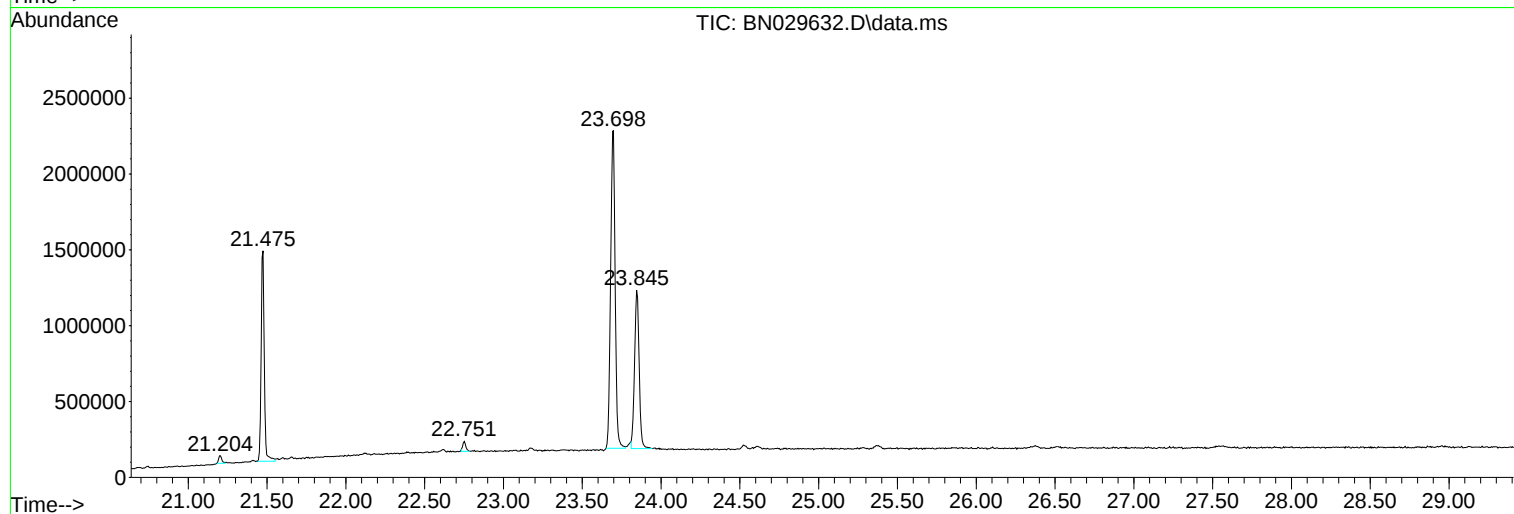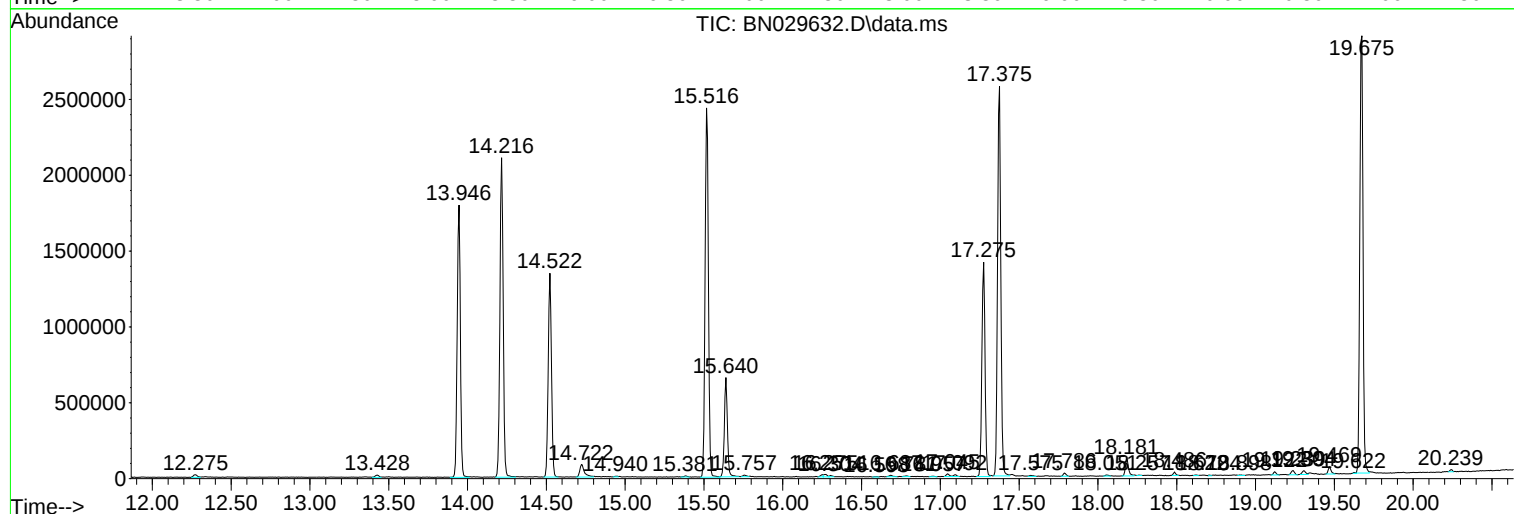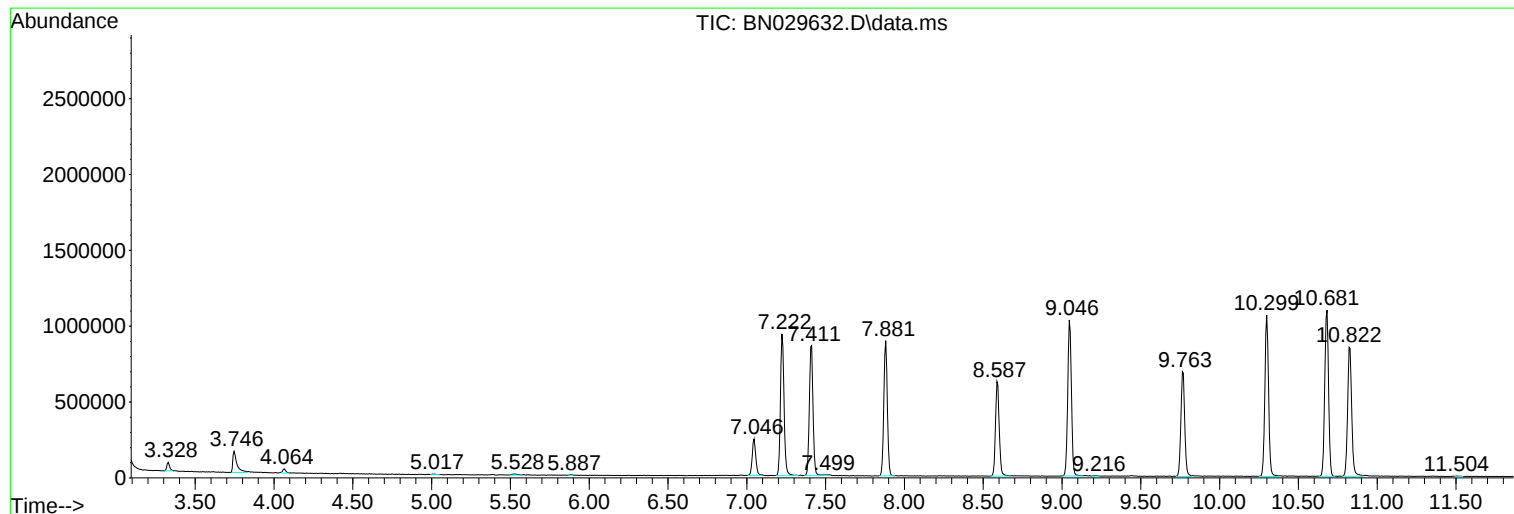

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029632.D
Acq On : 10 Feb 2024 04:57
Operator : MA/JU
Sample : P1398-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029632.D
Acq On : 10 Feb 2024 04:57
Operator : MA/JU
Sample : P1398-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc