

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029635.D
 Acq On : 10 Feb 2024 06:45
 Operator : MA/JU
 Sample : P1398-19
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	47	rBV	53667	66811	1.68%	0.147%
2	3.740	108	111	127	rBV	231065	398407	10.00%	0.875%
3	4.064	162	166	171	rVB2	23891	30031	0.75%	0.066%
4	5.381	386	390	395	rVB6	3321	5706	0.14%	0.013%
5	5.511	409	412	415	rBV5	4912	7638	0.19%	0.017%
6	5.881	473	475	480	rVB4	5236	6337	0.16%	0.014%
7	5.940	480	485	490	rVB8	5101	9631	0.24%	0.021%
8	6.963	654	659	664	rVB4	3696	7144	0.18%	0.016%
9	7.046	666	673	680	rBV	264404	418608	10.51%	0.919%
10	7.222	696	703	723	rVB	1030112	1616130	40.57%	3.549%
11	7.405	727	734	745	rBV	949470	1500202	37.66%	3.295%
12	7.505	746	751	753	rBV5	3906	6817	0.17%	0.015%
13	7.675	773	780	790	rBV2	16896	36385	0.91%	0.080%
14	7.881	808	815	825	rBV	823453	1313219	32.97%	2.884%
15	8.587	928	935	947	rBV	720615	1144618	28.73%	2.514%
16	9.046	1005	1013	1027	rBV	1135695	1848224	46.40%	4.059%
17	9.763	1128	1135	1150	rBV	790039	1317514	33.07%	2.893%
18	10.299	1218	1226	1235	rBV	1160102	1919945	48.20%	4.217%
19	10.675	1282	1290	1298	rBV	1010441	1762593	44.25%	3.871%
20	10.822	1305	1315	1330	rBV	1123762	1962163	49.26%	4.309%
21	12.275	1553	1562	1567	rBV2	19167	35562	0.89%	0.078%
22	13.151	1706	1711	1718	rVB2	13721	22832	0.57%	0.050%
23	13.428	1753	1758	1765	rVB	22040	33477	0.84%	0.074%
24	13.498	1765	1770	1773	rBV6	4071	6457	0.16%	0.014%
25	13.945	1839	1846	1857	rBV	1935586	2673122	67.11%	5.871%
26	14.216	1884	1892	1905	rBV	2322192	3339028	83.82%	7.333%
27	14.522	1936	1944	1956	rBV	1296152	1896699	47.61%	4.165%
28	14.722	1973	1978	1991	rBV	83881	173748	4.36%	0.382%
29	15.334	2077	2082	2084	rBV5	2771	4131	0.10%	0.009%
30	15.516	2106	2113	2126	rBV	2638098	3821727	95.94%	8.393%
31	15.639	2128	2134	2147	rVV	650809	895075	22.47%	1.966%
32	15.757	2150	2154	2161	rVB5	11969	18994	0.48%	0.042%
33	16.092	2206	2211	2213	rBV4	3107	4183	0.11%	0.009%
34	16.304	2243	2247	2251	rVB4	8091	11385	0.29%	0.025%
35	17.275	2405	2412	2422	rBV	1333840	1875027	47.07%	4.118%
36	17.375	2422	2429	2444	rVV	2669418	3844742	96.52%	8.444%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029635.D
 Acq On : 10 Feb 2024 06:45
 Operator : MA/JU
 Sample : P1398-19
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	17.580	2460	2464	2466	rBV4	4224	5457	0.14%	0.012%
38	17.669	2476	2479	2482	rBV5	3758	4945	0.12%	0.011%
39	17.951	2523	2527	2532	rBV8	2777	5149	0.13%	0.011%
40	18.180	2560	2566	2571	rBV2	31006	45894	1.15%	0.101%
41	18.622	2637	2641	2644	rBV5	6087	7245	0.18%	0.016%
42	19.104	2718	2723	2724	rBV4	2917	5277	0.13%	0.012%
43	19.233	2741	2745	2752	rBV2	27210	40244	1.01%	0.088%
44	19.304	2753	2757	2761	rVV2	22959	31720	0.80%	0.070%
45	19.469	2781	2785	2789	rBV3	27677	36821	0.92%	0.081%
46	19.622	2809	2811	2813	rBV3	7656	7413	0.19%	0.016%
47	19.669	2813	2819	2829	rVV	2897220	3983439	100.00%	8.748%
48	21.469	3120	3125	3140	rBV	1293887	1671910	41.97%	3.672%
49	23.692	3495	3503	3515	rBV	1899115	3831825	96.19%	8.415%
50	23.839	3522	3528	3539	rVB	881812	1822175	45.74%	4.002%




Sum of corrected areas: 45533826

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029635.D
Acq On : 10 Feb 2024 06:45
Operator : MA/JU
Sample : P1398-19
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

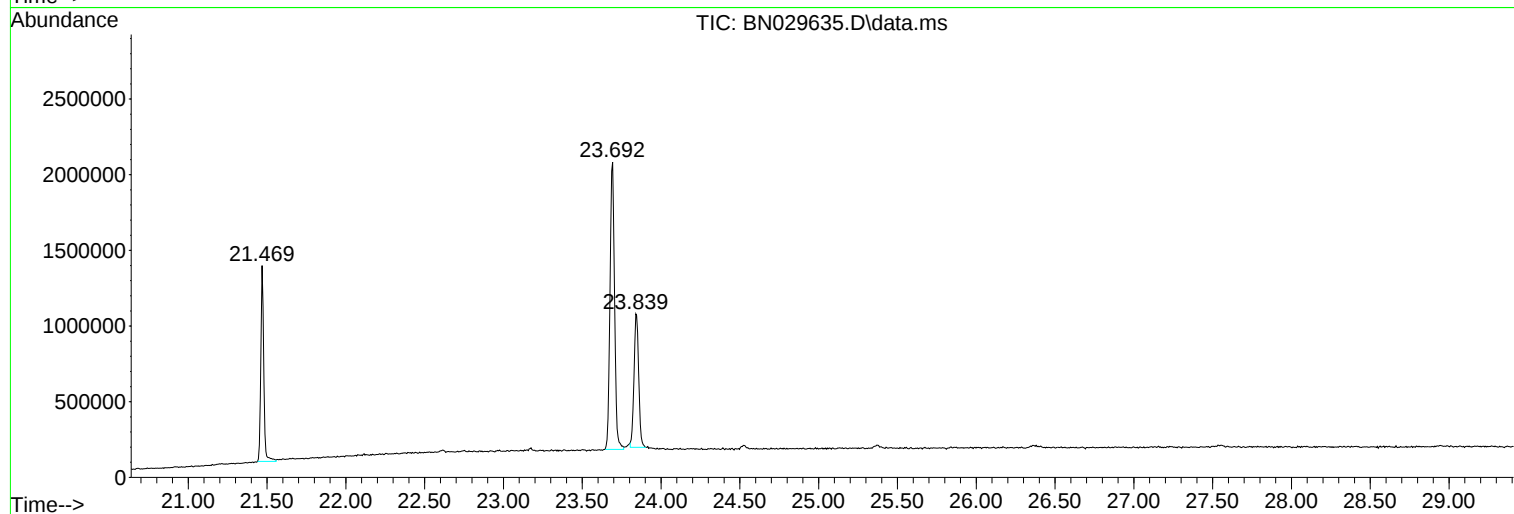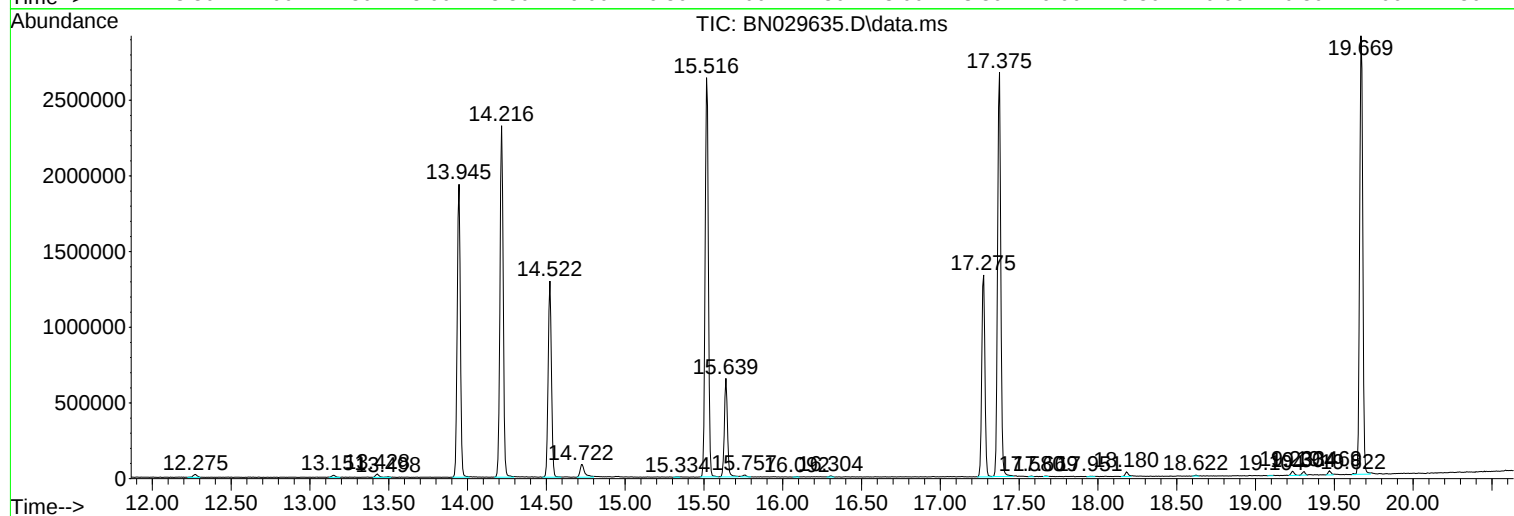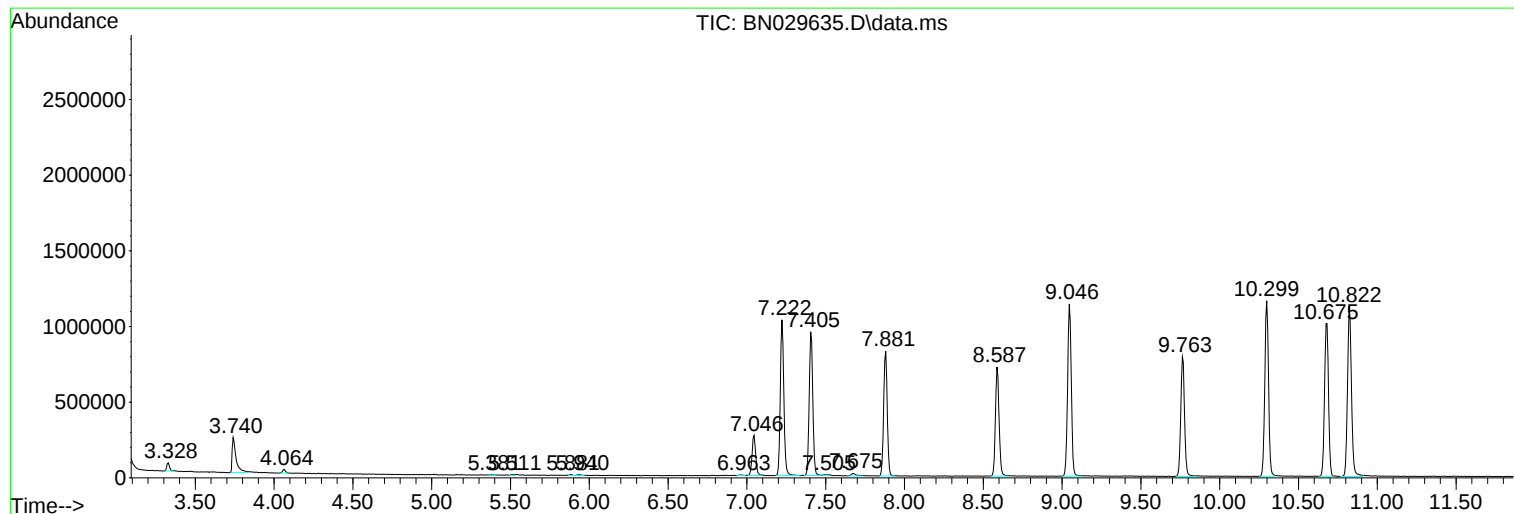

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029635.D
Acq On : 10 Feb 2024 06:45
Operator : MA/JU
Sample : P1398-19
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029635.D
Acq On : 10 Feb 2024 06:45
Operator : MA/JU
Sample : P1398-19
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------