

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029636.D
 Acq On : 10 Feb 2024 07:21
 Operator : MA/JU
 Sample : P1399-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029636.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	37	40	49	rVB	54202	75719	1.67%	0.152%
2	3.740	109	111	127	rBV	147373	264662	5.83%	0.530%
3	4.064	162	166	170	rVB	17721	25258	0.56%	0.051%
4	4.581	250	254	260	rBV2	16971	22793	0.50%	0.046%
5	5.005	325	326	329	rVB3	6091	4836	0.11%	0.010%
6	6.052	502	504	510	rVB7	3432	4829	0.11%	0.010%
7	7.046	666	673	681	rVV	274739	448953	9.88%	0.899%
8	7.222	696	703	715	rBV	1072723	1680543	36.99%	3.365%
9	7.405	726	734	745	rBV	1013268	1593108	35.07%	3.190%
10	7.493	745	749	753	rVV5	5421	8082	0.18%	0.016%
11	7.616	764	770	775	rVB3	38548	60134	1.32%	0.120%
12	7.881	807	815	824	rBV	862660	1410717	31.05%	2.825%
13	8.311	882	888	892	rVB8	2490	6150	0.14%	0.012%
14	8.505	916	921	925	rVB7	6286	9757	0.21%	0.020%
15	8.587	927	935	946	rBV	777089	1235327	27.19%	2.473%
16	8.687	946	952	959	rVV3	20184	43961	0.97%	0.088%
17	8.987	997	1003	1006	rBV2	16528	26085	0.57%	0.052%
18	9.046	1006	1013	1027	rVB	1190168	1935860	42.61%	3.876%
19	9.763	1128	1135	1148	rBV	826710	1371904	30.20%	2.747%
20	10.299	1218	1226	1240	rBV	1220353	2060234	45.35%	4.125%
21	10.546	1262	1268	1271	rBV6	6175	9600	0.21%	0.019%
22	10.675	1282	1290	1306	rVB	1135137	1912324	42.10%	3.829%
23	10.822	1308	1315	1333	rBV	542959	960600	21.15%	1.923%
24	11.340	1396	1403	1413	rVB5	9551	21070	0.46%	0.042%
25	11.440	1416	1420	1424	rBV6	3681	6412	0.14%	0.013%
26	12.016	1513	1518	1524	rBV2	17861	34733	0.76%	0.070%
27	12.269	1550	1561	1567	rVB4	19930	51314	1.13%	0.103%
28	12.340	1570	1573	1578	rVB4	5380	7915	0.17%	0.016%
29	12.481	1594	1597	1603	rVB7	3849	6528	0.14%	0.013%
30	12.704	1629	1635	1640	rBV5	11371	18490	0.41%	0.037%
31	12.787	1646	1649	1652	rBV4	5326	7412	0.16%	0.015%
32	12.869	1662	1663	1668	rVB5	3951	5087	0.11%	0.010%
33	13.146	1706	1710	1717	rVB2	8126	12344	0.27%	0.025%
34	13.357	1741	1746	1750	rBV5	7839	12021	0.26%	0.024%
35	13.428	1750	1758	1764	rVV4	26067	49144	1.08%	0.098%
36	13.487	1764	1768	1773	rVB6	3607	6529	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029636.D
 Acq On : 10 Feb 2024 07:21
 Operator : MA/JU
 Sample : P1399-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	13.946	1838	1846	1858	rBV	2039173	2870064	63.18%	5.747%
38	14.093	1867	1871	1874	rVB6	4773	6798	0.15%	0.014%
39	14.216	1885	1892	1902	rBV	2408278	3542076	77.97%	7.092%
40	14.293	1902	1905	1910	rVB3	18409	25974	0.57%	0.052%
41	14.522	1934	1944	1953	rBV	1375393	2178353	47.95%	4.362%
42	14.693	1969	1973	1974	rVV3	8832	9836	0.22%	0.020%
43	14.728	1974	1979	1996	rVB	126170	237349	5.22%	0.475%
44	15.328	2076	2081	2085	rBV2	8322	14747	0.32%	0.030%
45	15.475	2099	2106	2107	rBV	29427	40387	0.89%	0.081%
46	15.516	2107	2113	2119	rVV	2866815	4094508	90.13%	8.198%
47	15.563	2119	2121	2127	rVV6	17927	27840	0.61%	0.056%
48	15.640	2127	2134	2147	rVV	747121	1047895	23.07%	2.098%
49	15.757	2150	2154	2164	rVB7	14834	25664	0.56%	0.051%
50	16.098	2206	2212	2218	rBV2	37647	55925	1.23%	0.112%
51	16.216	2227	2232	2234	rBV6	5035	7592	0.17%	0.015%
52	16.298	2243	2246	2253	rVB8	9729	15204	0.33%	0.030%
53	16.469	2272	2275	2278	rBV5	3785	5052	0.11%	0.010%
54	16.687	2307	2312	2316	rVB6	4800	7931	0.17%	0.016%
55	16.957	2355	2358	2362	rVB6	4541	5287	0.12%	0.011%
56	17.081	2372	2379	2385	rVV4	33296	54233	1.19%	0.109%
57	17.275	2405	2412	2421	rBV	1443292	2072483	45.62%	4.150%
58	17.375	2421	2429	2441	rBV2	2846245	4166010	91.71%	8.341%
59	17.575	2458	2463	2468	rBV2	16359	24657	0.54%	0.049%
60	17.669	2477	2479	2484	rBV6	4843	5766	0.13%	0.012%
61	17.822	2499	2505	2513	rBV	228170	324575	7.14%	0.650%
62	18.034	2537	2541	2551	rBV8	9466	22586	0.50%	0.045%
63	18.181	2561	2566	2573	rBV	60951	90712	2.00%	0.182%
64	18.257	2576	2579	2581	rVV2	8669	12218	0.27%	0.024%
65	18.286	2581	2584	2588	rVV6	8881	15265	0.34%	0.031%
66	18.339	2591	2593	2598	rVB6	6772	8901	0.20%	0.018%
67	18.622	2637	2641	2644	rBV4	11102	10981	0.24%	0.022%
68	18.775	2664	2667	2668	rBV3	4834	4563	0.10%	0.009%
69	18.951	2693	2697	2702	rBV2	20886	30828	0.68%	0.062%
70	19.075	2713	2718	2730	rBV2	40426	70293	1.55%	0.141%
71	19.233	2740	2745	2750	rBV2	36570	50692	1.12%	0.101%
72	19.304	2753	2757	2762	rBV	30937	42288	0.93%	0.085%
73	19.469	2781	2785	2789	rBV3	28738	39164	0.86%	0.078%
74	19.622	2808	2811	2813	rBV3	8102	7556	0.17%	0.015%
75	19.669	2813	2819	2828	rVV	3179543	4421137	97.32%	8.852%
76	19.739	2828	2831	2836	rVB6	14403	25078	0.55%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029636.D
Acq On : 10 Feb 2024 07:21
Operator : MA/JU
Sample : P1399-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

77	21.198	3076	3079	3084	rBV6	37176	52528	1.16%	0.105%
78	21.469	3120	3125	3137	rBV2	1474992	1983830	43.67%	3.972%
79	23.692	3495	3503	3514	rBV	2291945	4542703	100.00%	9.096%
80	23.845	3522	3529	3545	rVB2	1064482	2236044	49.22%	4.477%


Sum of corrected areas: 49944008

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029636.D
Acq On : 10 Feb 2024 07:21
Operator : MA/JU
Sample : P1399-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

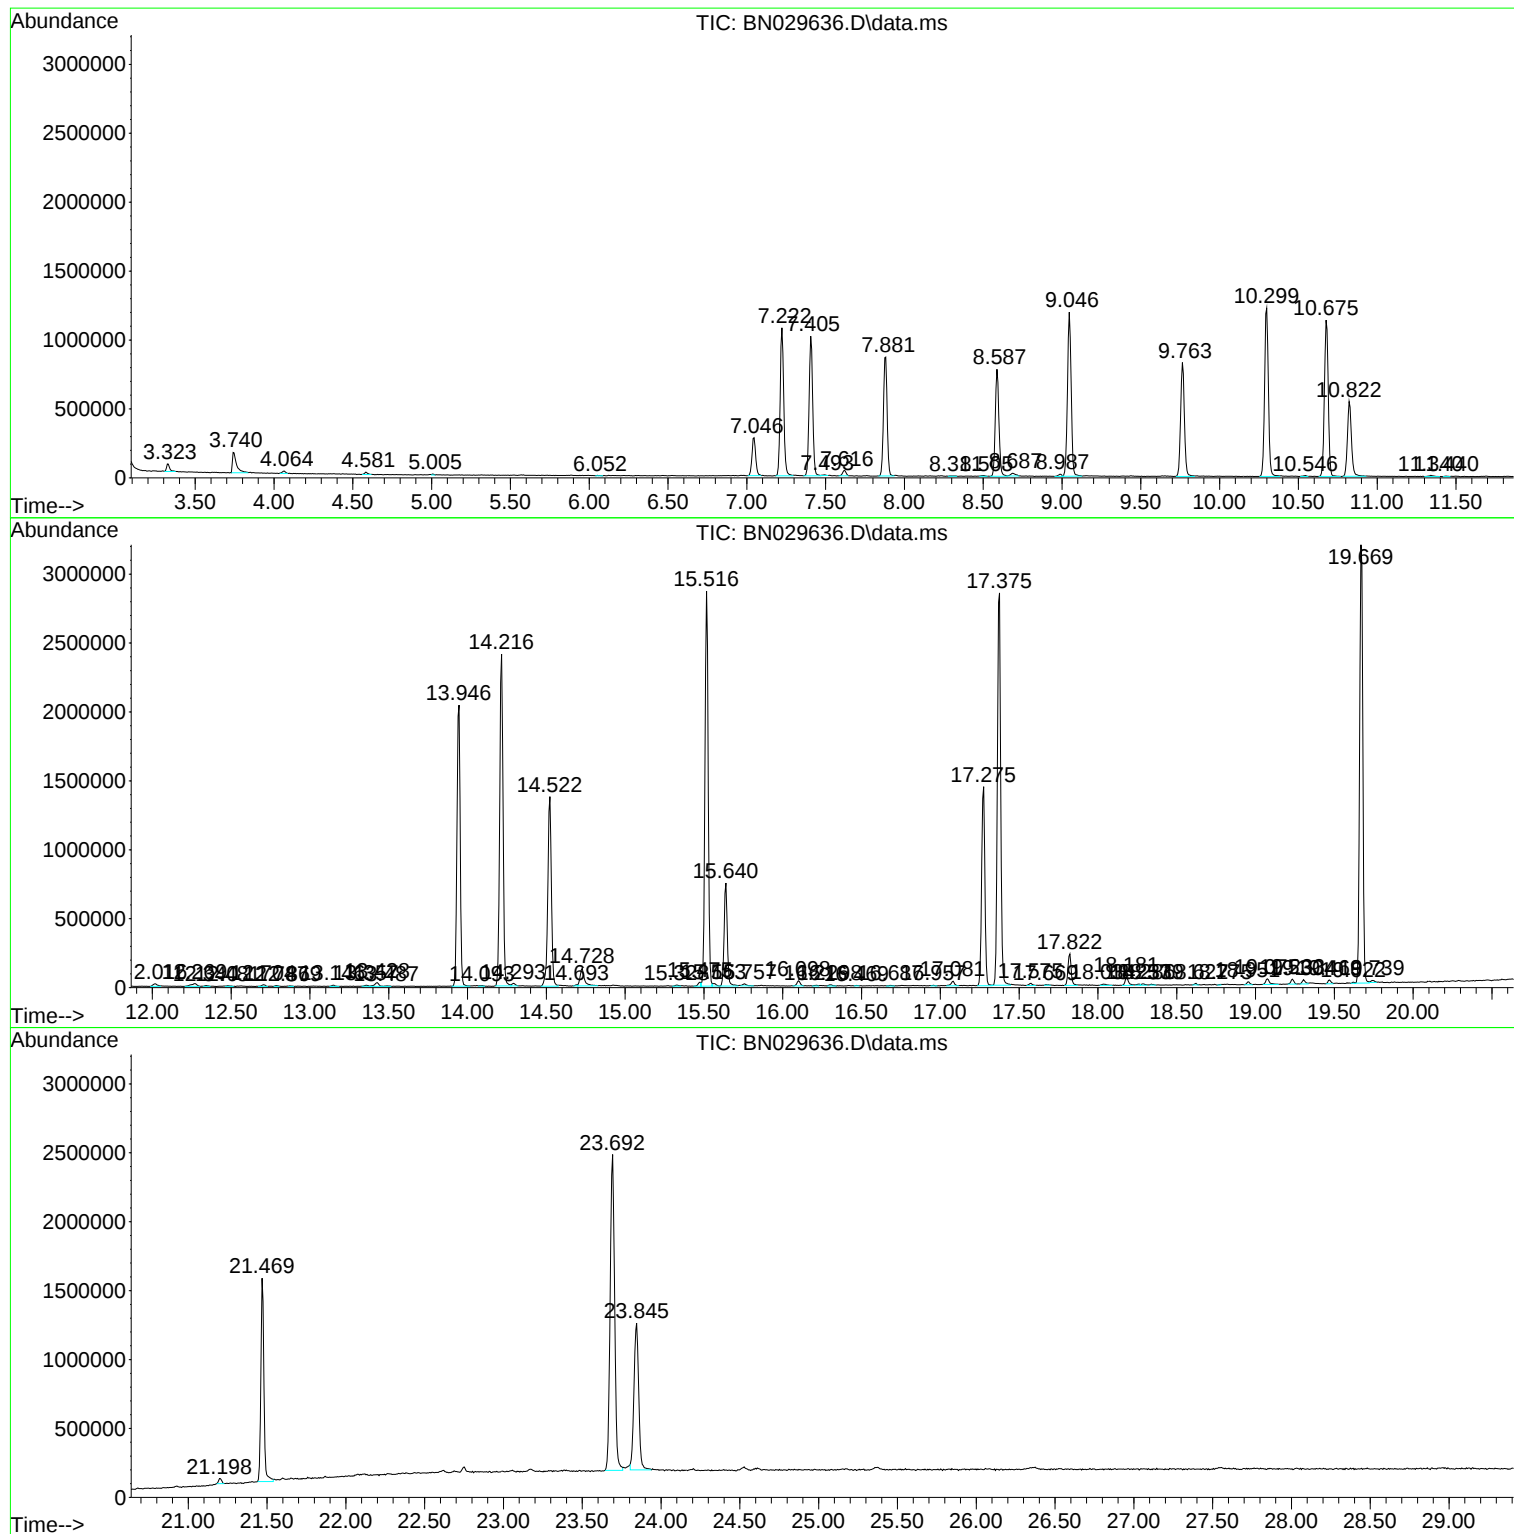

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029636.D
Acq On : 10 Feb 2024 07:21
Operator : MA/JU
Sample : P1399-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.822	3.13 ng/ul	324575	Phenanthrene-d10	17.275

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Morpholine	87	C4H9NO	000110-91-8	38
2			Morpholine	87	C4H9NO	000110-91-8	35
3			Morpholine, 4,4'-(1,2-dioxo-1,2-...	228	C10H16N2O4	006342-79-6	27
4			N-(2-Morpholino-2-oxoethyl)-4-ni...	283	C10H13N5O5	328071-10-9	25
5			1,6-Anhydro-2,3-dideoxy-.beta.-D...	130	C6H10O3	039682-47-8	16

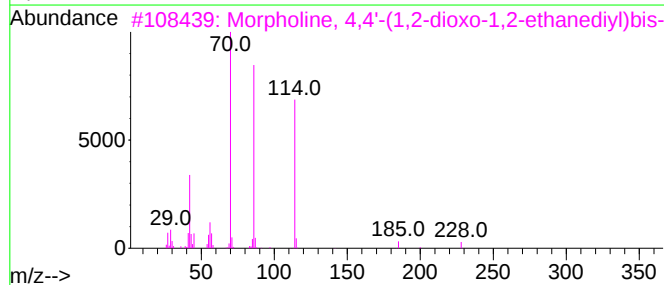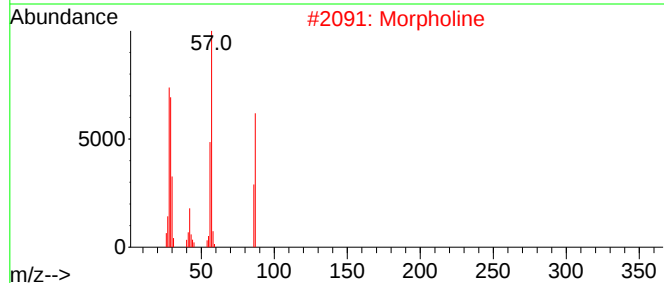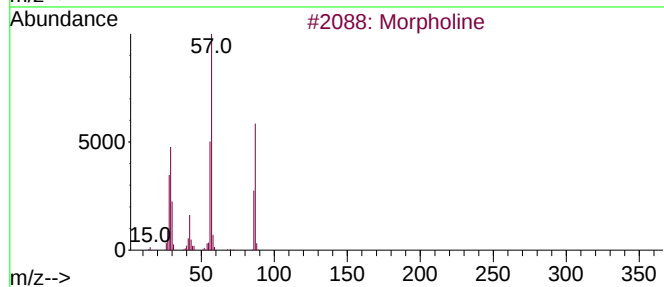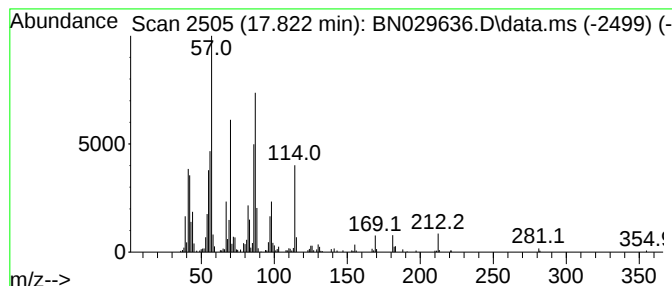

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029636.D
Acq On : 10 Feb 2024 07:21
Operator : MA/JU
Sample : P1399-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	17.822	3.1	ng/u1	324575	4	17.275	2072480	20.0