

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029640.D
 Acq On : 10 Feb 2024 09:46
 Operator : MA/JU
 Sample : P1399-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	47	rBV	55083	72427	1.63%	0.158%
2	3.740	107	111	127	rBV	252943	427648	9.65%	0.936%
3	4.064	162	166	177	rVB	18746	33224	0.75%	0.073%
4	5.005	324	326	333	rVB5	3836	6890	0.16%	0.015%
5	5.522	410	414	415	rBV4	4062	5382	0.12%	0.012%
6	5.881	471	475	480	rBV7	5074	8655	0.20%	0.019%
7	6.969	657	660	664	rVB6	4201	6759	0.15%	0.015%
8	7.046	666	673	686	rVB	294510	475012	10.72%	1.040%
9	7.222	696	703	716	rBV	1035354	1637834	36.95%	3.584%
10	7.405	727	734	746	rBV	987489	1583035	35.71%	3.464%
11	7.499	746	750	752	rVV4	4700	5464	0.12%	0.012%
12	7.875	804	814	822	rBV	707490	1150026	25.94%	2.517%
13	7.940	822	825	830	rVB6	4860	8034	0.18%	0.018%
14	8.587	927	935	951	rBV	785334	1252582	28.26%	2.741%
15	9.046	1005	1013	1025	rVV	1135630	1852492	41.79%	4.054%
16	9.151	1027	1031	1036	rVB6	5692	9977	0.23%	0.022%
17	9.763	1127	1135	1146	rBV	805163	1329886	30.00%	2.910%
18	10.298	1216	1226	1239	rBV	1172764	1990489	44.90%	4.356%
19	10.404	1242	1244	1250	rVB5	3535	5466	0.12%	0.012%
20	10.675	1282	1290	1298	rBV	899540	1538140	34.70%	3.366%
21	10.822	1306	1315	1328	rBV	858232	1517888	34.24%	3.322%
22	11.346	1400	1404	1409	rVB6	2880	4929	0.11%	0.011%
23	11.498	1424	1430	1432	rBV3	5235	8090	0.18%	0.018%
24	12.269	1556	1561	1567	rVB2	19260	34666	0.78%	0.076%
25	13.151	1707	1711	1717	rVB	14875	22118	0.50%	0.048%
26	13.422	1752	1757	1762	rBV5	10875	16487	0.37%	0.036%
27	13.945	1839	1846	1857	rBV	1877037	2720874	61.38%	5.954%
28	14.216	1883	1892	1902	rBV	2282139	3365713	75.93%	7.365%
29	14.522	1937	1944	1952	rBV	1095134	1622439	36.60%	3.551%
30	14.728	1972	1979	1990	rBV	109941	218676	4.93%	0.479%
31	14.945	2010	2016	2023	rVB10	2708	6371	0.14%	0.014%
32	15.516	2106	2113	2119	rBV	2792115	3948527	89.08%	8.641%
33	15.563	2119	2121	2127	rVV2	35827	42830	0.97%	0.094%
34	15.639	2127	2134	2148	rVV	709822	996624	22.48%	2.181%
35	15.757	2148	2154	2158	rVB5	11966	21174	0.48%	0.046%
36	16.304	2243	2247	2253	rBV4	8261	12519	0.28%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029640.D
 Acq On : 10 Feb 2024 09:46
 Operator : MA/JU
 Sample : P1399-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	17.275	2405	2412	2420	rBV	1128421	1642871	37.06%	3.595%
38	17.369	2422	2428	2442	rBV2	2753677	4086188	92.18%	8.942%
39	18.180	2562	2566	2571	rBV6	18001	26899	0.61%	0.059%
40	18.622	2637	2641	2646	rVB6	7406	7506	0.17%	0.016%
41	19.233	2741	2745	2750	rVB2	31168	41890	0.95%	0.092%
42	19.304	2753	2757	2762	rBV2	26703	40455	0.91%	0.089%
43	19.345	2762	2764	2769	rBV5	3357	5964	0.13%	0.013%
44	19.469	2781	2785	2789	rBV5	16520	21957	0.50%	0.048%
45	19.622	2807	2811	2813	rBV4	6712	9986	0.23%	0.022%
46	19.669	2813	2819	2827	rVV	3212500	4255871	96.01%	9.313%
47	21.468	3120	3125	3133	rBV	1145346	1511534	34.10%	3.308%
48	23.692	3495	3503	3515	rBV2	2171568	4432742	100.00%	9.701%
49	23.845	3522	3529	3538	rVB	820944	1652792	37.29%	3.617%




Sum of corrected areas: 45696002

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029640.D
Acq On : 10 Feb 2024 09:46
Operator : MA/JU
Sample : P1399-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

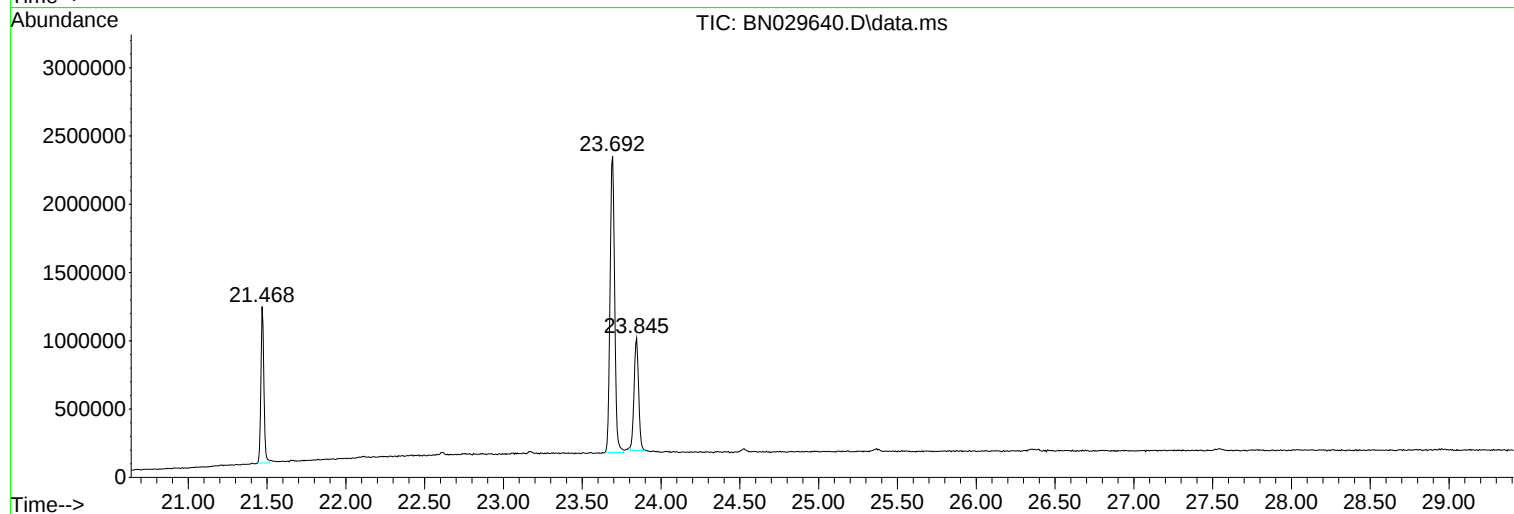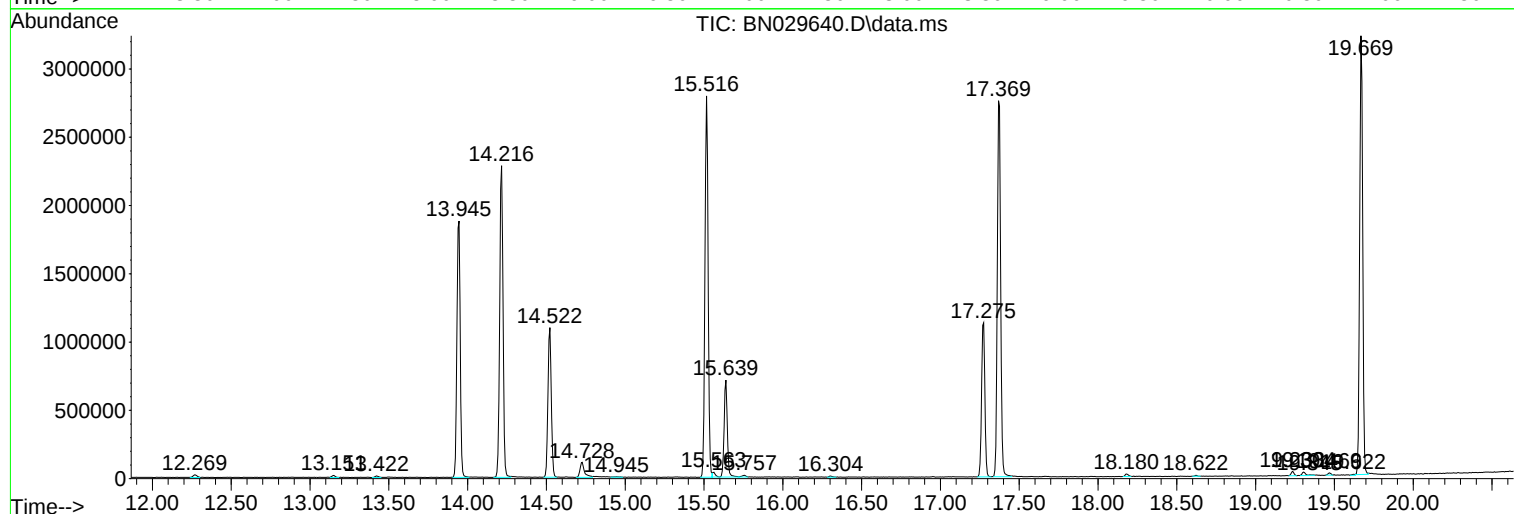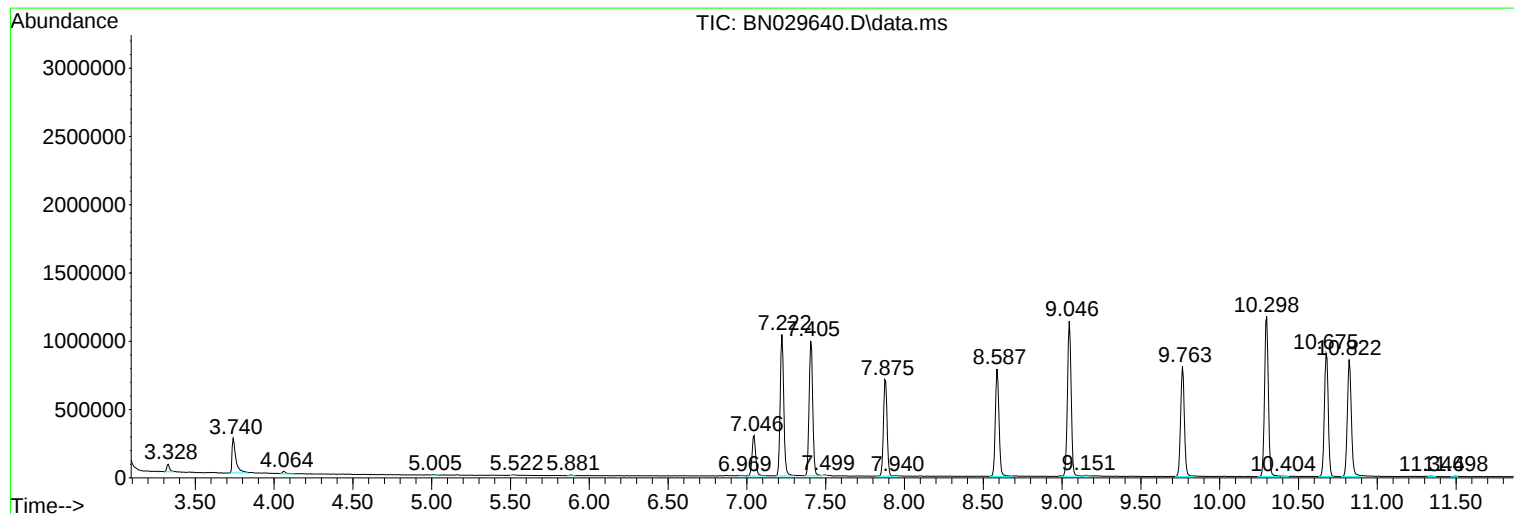

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029640.D
Acq On : 10 Feb 2024 09:46
Operator : MA/JU
Sample : P1399-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029640.D
Acq On : 10 Feb 2024 09:46
Operator : MA/JU
Sample : P1399-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc