

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029641.D
 Acq On : 10 Feb 2024 10:22
 Operator : MA/JU
 Sample : P1399-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	37	40	51	rVB	54438	75383	1.75%	0.171%
2	3.740	107	111	130	rBV	218578	383327	8.92%	0.867%
3	4.064	162	166	169	rVB	15944	20359	0.47%	0.046%
4	6.957	655	658	663	rBV7	4120	6762	0.16%	0.015%
5	7.046	666	673	683	rVV	256166	415058	9.66%	0.939%
6	7.222	696	703	721	rBV	941031	1508442	35.11%	3.412%
7	7.405	724	734	744	rBV	922123	1445891	33.66%	3.271%
8	7.493	746	749	754	rVB6	5697	9491	0.22%	0.021%
9	7.875	807	814	822	rBV	747069	1209620	28.16%	2.736%
10	8.587	928	935	952	rBV	695959	1113194	25.91%	2.518%
11	9.046	1005	1013	1025	rBV	1043675	1699690	39.56%	3.845%
12	9.763	1127	1135	1150	rBV	726474	1196809	27.86%	2.707%
13	10.298	1215	1226	1238	rBV	1070328	1810343	42.14%	4.095%
14	10.675	1283	1290	1298	rBV	961890	1603592	37.33%	3.628%
15	10.822	1306	1315	1328	rBV	859961	1508910	35.12%	3.413%
16	11.345	1401	1404	1409	rVB6	2920	4438	0.10%	0.010%
17	12.198	1546	1549	1554	rVB6	3083	4485	0.10%	0.010%
18	12.275	1556	1562	1569	rVV2	16079	30980	0.72%	0.070%
19	13.151	1706	1711	1715	rVB4	8252	13361	0.31%	0.030%
20	13.428	1751	1758	1762	rBV4	14483	23945	0.56%	0.054%
21	13.492	1765	1769	1774	rVV5	3784	5099	0.12%	0.012%
22	13.945	1839	1846	1858	rBV	1807102	2578060	60.01%	5.832%
23	14.216	1884	1892	1903	rBV	2136147	3120955	72.65%	7.060%
24	14.522	1937	1944	1954	rVV	1211896	1743741	40.59%	3.945%
25	14.722	1972	1978	1989	rBV	101533	206556	4.81%	0.467%
26	15.322	2076	2080	2085	rBV6	3345	6098	0.14%	0.014%
27	15.516	2106	2113	2120	rBV	2665690	3727320	86.76%	8.432%
28	15.639	2128	2134	2146	rBV	659125	913538	21.27%	2.067%
29	15.757	2150	2154	2158	rVB5	12595	17894	0.42%	0.040%
30	16.298	2243	2246	2254	rVB7	7729	13077	0.30%	0.030%
31	16.951	2353	2357	2361	rBV7	4448	10058	0.23%	0.023%
32	17.269	2405	2411	2421	rBV	1214832	1792269	41.72%	4.055%
33	17.375	2421	2429	2442	rBV2	2588953	3830315	89.16%	8.665%
34	17.669	2475	2479	2483	rBV6	7366	11570	0.27%	0.026%
35	17.827	2501	2506	2508	rBV6	3842	5111	0.12%	0.012%
36	18.186	2562	2567	2573	rBV5	15707	26944	0.63%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029641.D
Acq On : 10 Feb 2024 10:22
Operator : MA/JU
Sample : P1399-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	18.622	2638	2641	2645	rVB4	11493	13165	0.31%	0.030%
38	18.810	2671	2673	2678	rVB6	3653	4881	0.11%	0.011%
39	19.233	2741	2745	2749	rBV3	30073	42566	0.99%	0.096%
40	19.304	2753	2757	2762	rBV	23056	32035	0.75%	0.072%
41	19.374	2768	2769	2774	rVB4	5695	7367	0.17%	0.017%
42	19.469	2781	2785	2791	rBV9	15536	29016	0.68%	0.066%
43	19.669	2813	2819	2827	rBV2	3074590	4173397	97.15%	9.441%
44	19.933	2862	2864	2866	rBV3	5742	4844	0.11%	0.011%
45	21.468	3120	3125	3132	rBV	1216037	1666029	38.78%	3.769%
46	23.692	3495	3503	3514	rBV	2159594	4295948	100.00%	9.718%
47	23.845	3522	3529	3537	rVB	911526	1842342	42.89%	4.168%


Sum of corrected areas: 44204275

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029641.D
Acq On : 10 Feb 2024 10:22
Operator : MA/JU
Sample : P1399-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

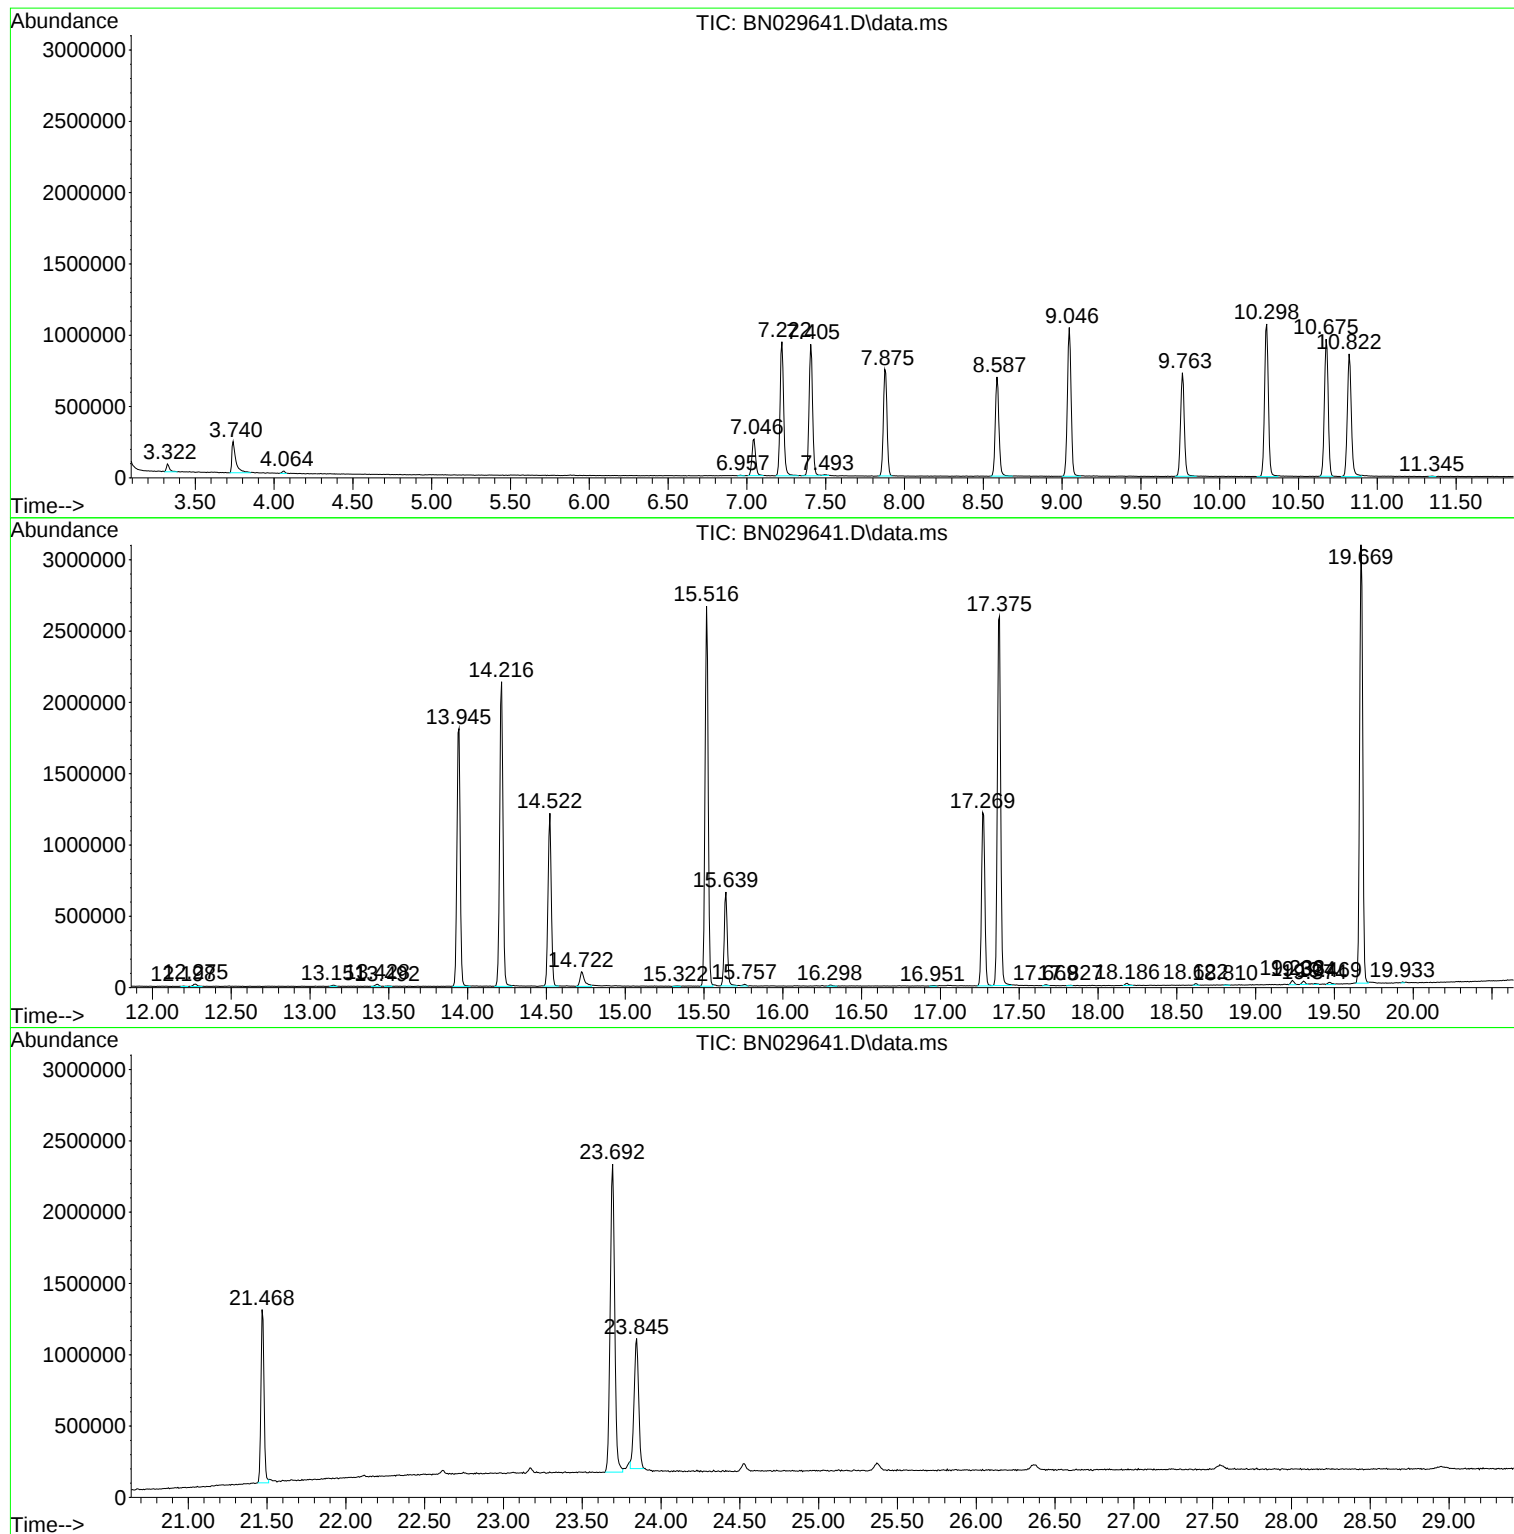

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029641.D
Acq On : 10 Feb 2024 10:22
Operator : MA/JU
Sample : P1399-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029641.D
Acq On : 10 Feb 2024 10:22
Operator : MA/JU
Sample : P1399-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc