

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029647.D
 Acq On : 10 Feb 2024 14:35
 Operator : MA/JU
 Sample : PB158925BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK925

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	48	rVB	84603	110555	2.97%	0.219%
2	3.734	106	110	136	rBV	976398	1519483	40.82%	3.011%
3	4.058	162	165	170	rVB	23401	31815	0.85%	0.063%
4	5.111	341	344	348	rBV6	2837	3776	0.10%	0.007%
5	7.046	666	673	683	rBV	1176987	1871707	50.29%	3.709%
6	7.222	696	703	718	rBV	986835	1544020	41.48%	3.059%
7	7.405	727	734	747	rBV	1195199	1872228	50.30%	3.710%
8	7.875	807	814	822	rBV	903955	1446037	38.85%	2.865%
9	8.587	927	935	945	rBV	1415090	2231806	59.96%	4.422%
10	9.046	1004	1013	1023	rBV	1101300	1796095	48.25%	3.559%
11	9.763	1125	1135	1146	rBV	829065	1360251	36.54%	2.695%
12	10.293	1218	1225	1237	rBV	1235070	2094823	56.28%	4.151%
13	10.675	1282	1290	1299	rBV	1236793	2028760	54.51%	4.020%
14	10.822	1307	1315	1329	rBV	1270059	2222906	59.72%	4.404%
15	12.269	1556	1561	1567	rBV2	18622	33259	0.89%	0.066%
16	12.487	1593	1598	1602	rVB8	1982	4051	0.11%	0.008%
17	13.422	1751	1757	1764	rVB3	10749	17660	0.47%	0.035%
18	13.940	1837	1845	1861	rBV	1909272	2682935	72.08%	5.316%
19	14.216	1885	1892	1902	rBV	2234221	3352564	90.07%	6.643%
20	14.522	1937	1944	1956	rBV	1512539	2251629	60.49%	4.461%
21	14.634	1958	1963	1964	rBV5	4043	4995	0.13%	0.010%
22	14.722	1971	1978	1996	rBV	625570	1027407	27.60%	2.036%
23	15.516	2106	2113	2126	rBV	2628280	3722143	100.00%	7.375%
24	15.639	2127	2134	2145	rVV	595869	852431	22.90%	1.689%
25	15.757	2149	2154	2159	rVB4	11395	18579	0.50%	0.037%
26	16.304	2243	2247	2253	rBV7	8425	12011	0.32%	0.024%
27	16.951	2350	2357	2362	rBV8	4184	6128	0.16%	0.012%
28	17.269	2405	2411	2422	rBV	1451175	2140969	57.52%	4.242%
29	17.369	2422	2428	2449	rVB2	2340401	3467686	93.16%	6.871%
30	18.181	2564	2566	2570	rBV5	4333	5142	0.14%	0.010%
31	19.233	2741	2745	2750	rBV3	24338	38445	1.03%	0.076%
32	19.304	2753	2757	2763	rVV2	20717	30714	0.83%	0.061%
33	19.386	2767	2771	2774	rBV5	9997	12603	0.34%	0.025%
34	19.622	2806	2811	2814	rBV3	31406	42009	1.13%	0.083%
35	19.669	2814	2819	2827	rVB	2562250	3411234	91.65%	6.759%
36	20.675	2988	2990	2994	rVB5	14166	14358	0.39%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029647.D
Acq On : 10 Feb 2024 14:35
Operator : MA/JU
Sample : PB158925BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK925

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	21.469	3120	3125	3133	rBV2	1336271	1782612	47.89%	3.532%
38	23.692	3495	3503	3517	rBV2	1701364	3431170	92.18%	6.798%
39	23.839	3522	3528	3540	rVB2	958505	1972706	53.00%	3.909%




Sum of corrected areas: 50469702

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029647.D
Acq On : 10 Feb 2024 14:35
Operator : MA/JU
Sample : PB158925BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

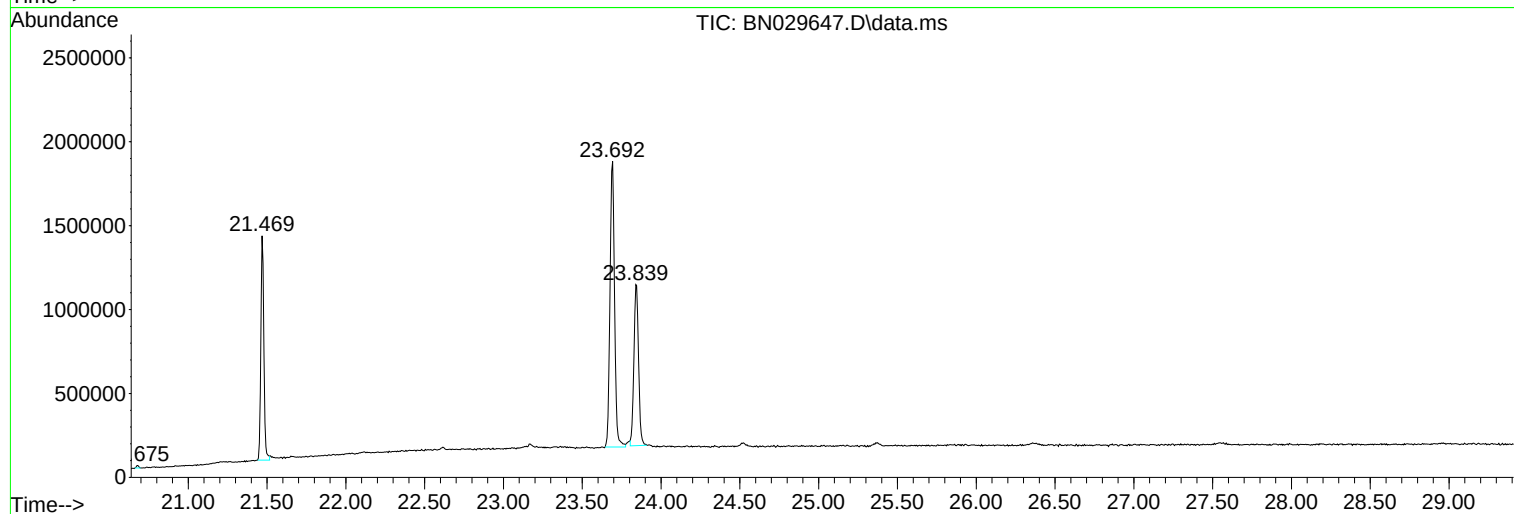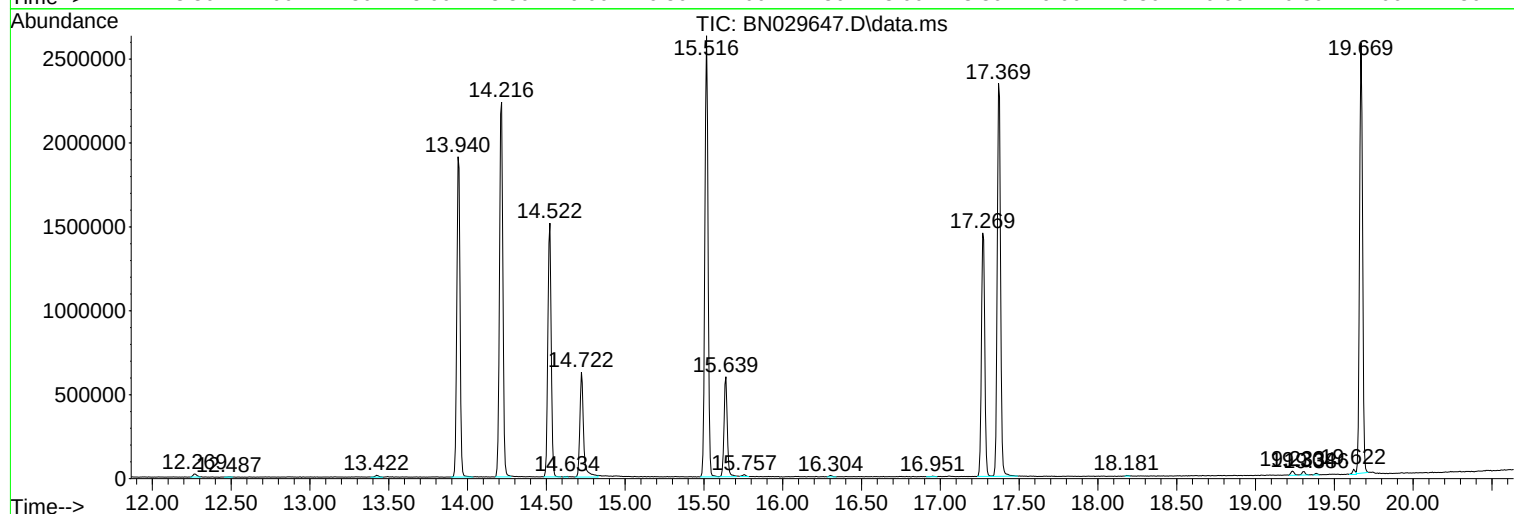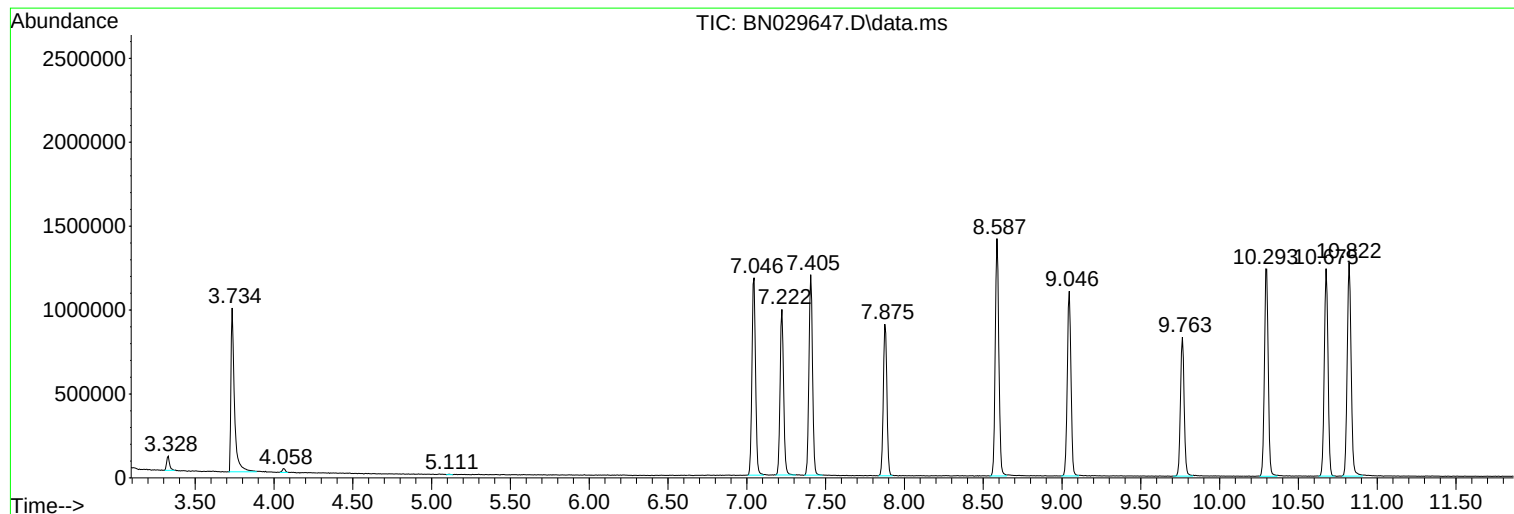

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029647.D
Acq On : 10 Feb 2024 14:35
Operator : MA/JU
Sample : PB158925BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029647.D
Acq On : 10 Feb 2024 14:35
Operator : MA/JU
Sample : PB158925BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK925

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------