

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029648.D
 Acq On : 10 Feb 2024 15:12
 Operator : MA/JU
 Sample : PB158927BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK927

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	53	rVB	87719	126258	3.29%	0.236%
2	3.734	106	110	127	rBV	1018918	1573152	40.96%	2.937%
3	4.064	162	166	174	rVB	23047	33274	0.87%	0.062%
4	7.046	666	673	687	rBV	1209702	1932282	50.31%	3.607%
5	7.222	696	703	714	rBV	1022272	1597723	41.60%	2.983%
6	7.405	727	734	748	rVB	1243847	1937757	50.45%	3.618%
7	7.875	807	814	823	rBV	1074423	1714364	44.64%	3.201%
8	8.587	928	935	946	rBV	1426049	2272557	59.17%	4.243%
9	9.046	1004	1013	1026	rBV	1142727	1860692	48.45%	3.474%
10	9.763	1127	1135	1145	rBV	847139	1389001	36.17%	2.593%
11	10.293	1218	1225	1243	rBV	1268116	2152048	56.03%	4.018%
12	10.675	1282	1290	1301	rBV	1409441	2367986	61.66%	4.421%
13	10.822	1305	1315	1329	rBV	1324673	2287344	59.56%	4.270%
14	12.269	1556	1561	1570	rVB2	22680	41241	1.07%	0.077%
15	13.422	1752	1757	1763	rBV3	19683	28967	0.75%	0.054%
16	13.940	1839	1845	1855	rBV	1966003	2789950	72.64%	5.209%
17	14.216	1884	1892	1904	rBV2	2284309	3423191	89.13%	6.391%
18	14.292	1904	1905	1912	rVB5	4224	5044	0.13%	0.009%
19	14.522	1937	1944	1951	rBV	1703109	2563722	66.75%	4.786%
20	14.722	1971	1978	1997	rBV	690767	1097240	28.57%	2.048%
21	14.940	2012	2015	2016	rBV3	4132	4183	0.11%	0.008%
22	15.516	2106	2113	2128	rBV	2758901	3840644	100.00%	7.170%
23	15.639	2128	2134	2147	rVV	629510	897128	23.36%	1.675%
24	15.751	2150	2153	2159	rVB4	12163	18296	0.48%	0.034%
25	16.298	2240	2246	2252	rBV6	8544	13729	0.36%	0.026%
26	16.951	2353	2357	2360	rBV6	5115	4889	0.13%	0.009%
27	17.063	2370	2376	2382	rBV7	4183	8983	0.23%	0.017%
28	17.269	2405	2411	2419	rBV	1678206	2466514	64.22%	4.605%
29	17.369	2422	2428	2444	rVB2	2551320	3652605	95.10%	6.819%
30	17.975	2528	2531	2534	rBV5	2714	4084	0.11%	0.008%
31	18.186	2564	2567	2573	rVB8	5053	7981	0.21%	0.015%
32	19.233	2741	2745	2750	rBV2	24252	31749	0.83%	0.059%
33	19.304	2752	2757	2761	rBV2	22723	31275	0.81%	0.058%
34	19.669	2813	2819	2829	rBV2	2652522	3589880	93.47%	6.702%
35	21.469	3120	3125	3137	rBV	1589969	2068007	53.85%	3.861%
36	23.686	3495	3502	3513	rBV	1764667	3458224	90.04%	6.456%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029648.D
Acq On : 10 Feb 2024 15:12
Operator : MA/JU
Sample : PB158927BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK927

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	23.839	3521	3528	3538	rVB	1094167	2273037	59.18%	4.244%
----	--------	------	------	------	-----	---------	---------	--------	--------


Sum of corrected areas: 53565001

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN029648\
Data File : BN029648.D
Acq On : 10 Feb 2024 15:12
Operator : MA/JU
Sample : PB158927BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK927

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

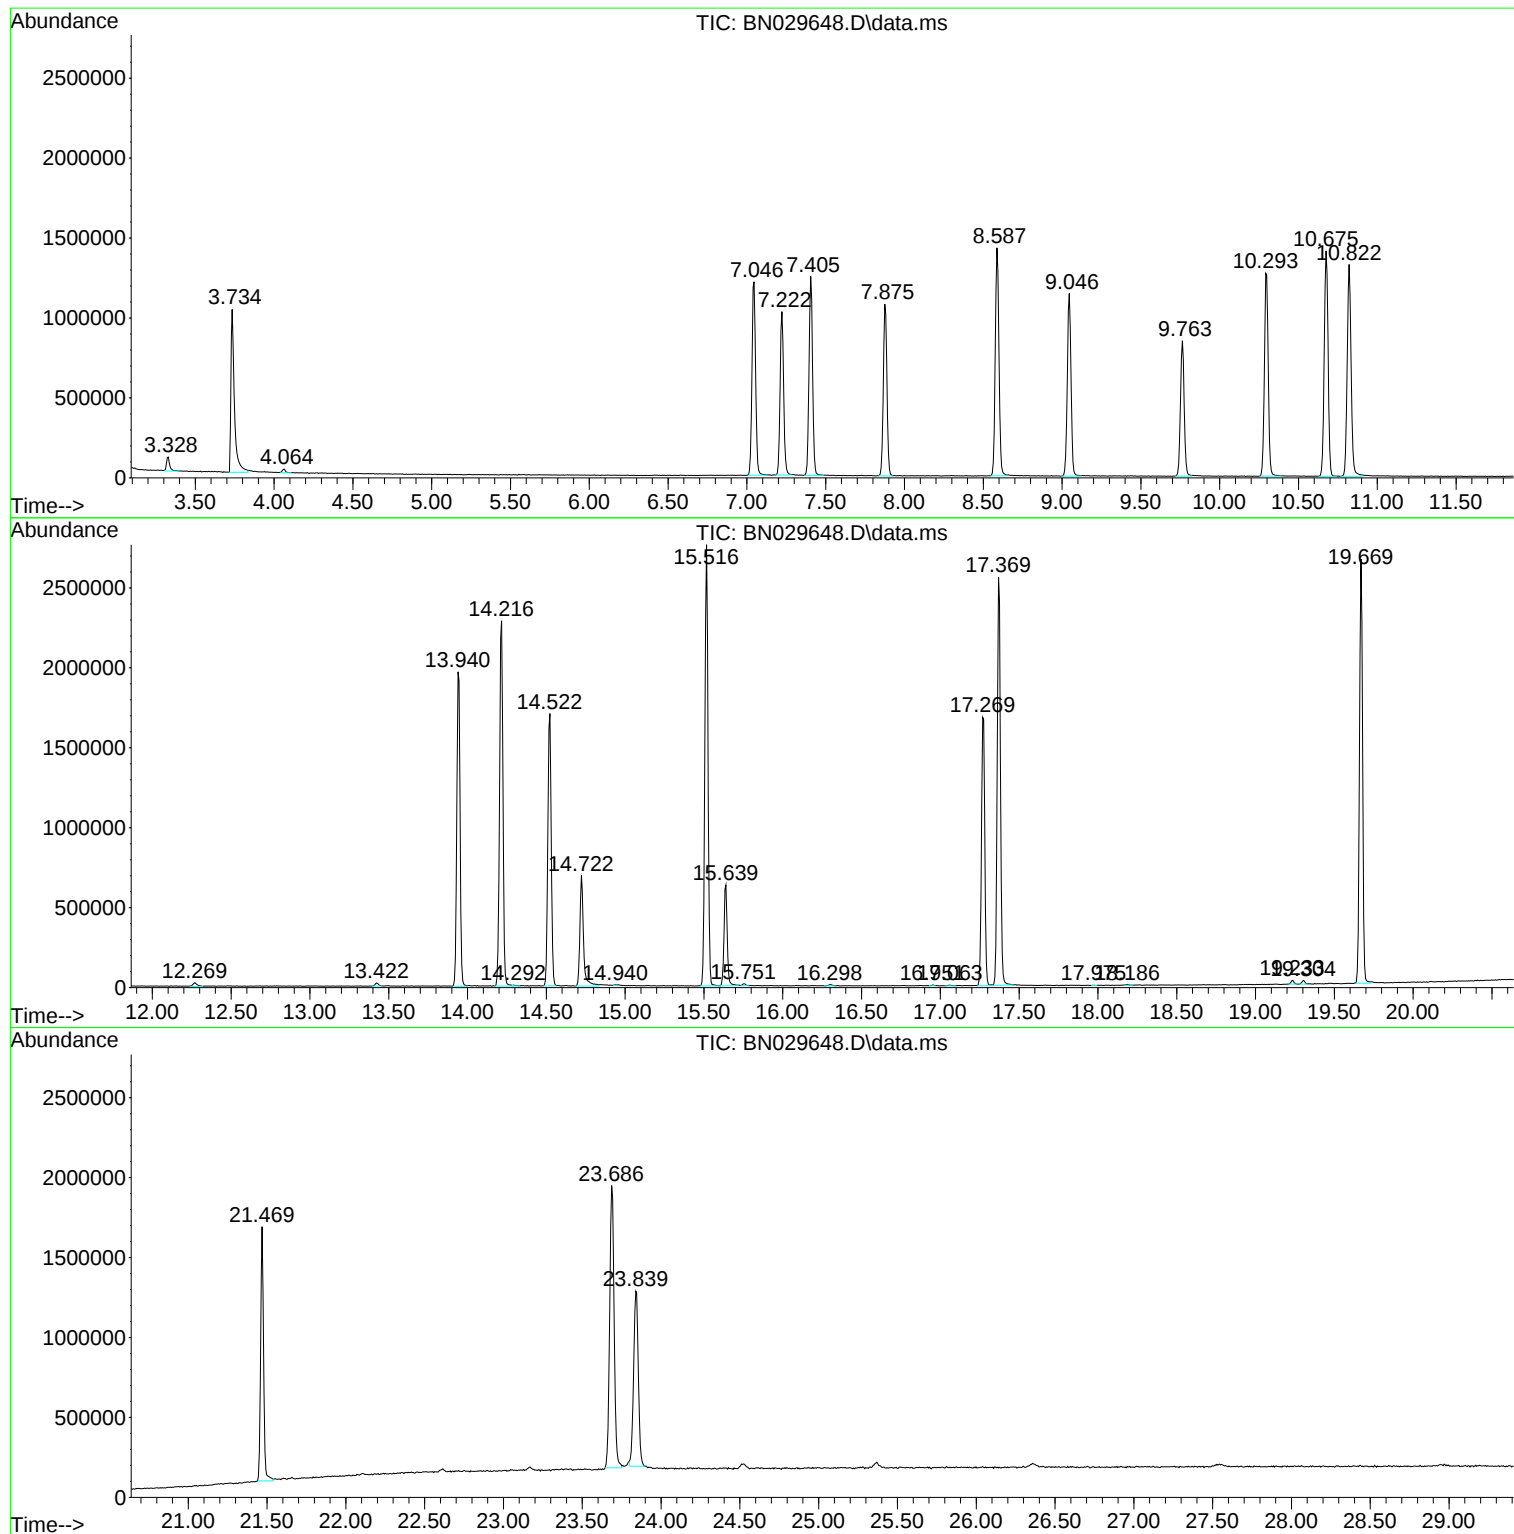

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029648.D
Acq On : 10 Feb 2024 15:12
Operator : MA/JU
Sample : PB158927BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK927

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029648.D
Acq On : 10 Feb 2024 15:12
Operator : MA/JU
Sample : PB158927BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK927

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------