

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029649.D
 Acq On : 10 Feb 2024 15:48
 Operator : MA/JU
 Sample : PB158929BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK929

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029649.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	52	rVB	87960	125872	3.32%	0.237%
2	3.734	106	110	129	rBV	1015553	1567992	41.35%	2.953%
3	4.064	162	166	170	rVB	19583	27184	0.72%	0.051%
4	6.999	660	665	666	rBV5	2378	4039	0.11%	0.008%
5	7.046	666	673	684	rVV	1216339	1936453	51.07%	3.646%
6	7.222	696	703	714	rBV	1032472	1602348	42.26%	3.017%
7	7.405	725	734	744	rBV	1230349	1934107	51.01%	3.642%
8	7.875	807	814	827	rBV	1039495	1668598	44.01%	3.142%
9	8.587	928	935	948	rBV	1446203	2279734	60.13%	4.293%
10	9.046	1005	1013	1024	rBV	1132554	1850687	48.81%	3.485%
11	9.763	1127	1135	1150	rBV	847896	1377654	36.33%	2.594%
12	10.293	1218	1225	1238	rBV	1254051	2127598	56.11%	4.006%
13	10.675	1282	1290	1298	rBV	1366790	2278054	60.08%	4.290%
14	10.822	1306	1315	1338	rBV	1309416	2289565	60.39%	4.311%
15	12.269	1553	1561	1567	rBV2	19511	34985	0.92%	0.066%
16	13.422	1753	1757	1762	rBV5	9799	15225	0.40%	0.029%
17	13.487	1765	1768	1772	rBV5	2883	4692	0.12%	0.009%
18	13.940	1837	1845	1856	rBV	1949470	2754499	72.65%	5.187%
19	14.210	1885	1891	1908	rBV	2247447	3358045	88.57%	6.323%
20	14.522	1937	1944	1957	rVB	1639900	2465327	65.02%	4.642%
21	14.628	1957	1962	1965	rBV5	4154	5519	0.15%	0.010%
22	14.722	1971	1978	1993	rBV	681909	1083264	28.57%	2.040%
23	14.951	2016	2017	2022	rVB5	6256	6854	0.18%	0.013%
24	15.516	2106	2113	2124	rBV	2675777	3791595	100.00%	7.140%
25	15.640	2128	2134	2146	rVV	608913	879085	23.19%	1.655%
26	15.751	2150	2153	2159	rVB4	12219	17449	0.46%	0.033%
27	15.928	2179	2183	2187	rVB7	2658	5114	0.13%	0.010%
28	16.298	2242	2246	2254	rBV7	6886	12312	0.32%	0.023%
29	17.051	2369	2374	2380	rBV7	3690	7152	0.19%	0.013%
30	17.269	2405	2411	2421	rBV	1729813	2403499	63.39%	4.526%
31	17.369	2422	2428	2444	rVV2	2532538	3634814	95.87%	6.844%
32	19.175	2732	2735	2737	rBV4	2988	4468	0.12%	0.008%
33	19.233	2741	2745	2751	rVV4	25405	38574	1.02%	0.073%
34	19.304	2753	2757	2763	rVB2	18858	31174	0.82%	0.059%
35	19.669	2813	2819	2827	rBV	2725016	3596940	94.87%	6.773%
36	21.469	3120	3125	3137	rBV	1572132	2048654	54.03%	3.858%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029649.D
Acq On : 10 Feb 2024 15:48
Operator : MA/JU
Sample : PB158929BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK929

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	23.686	3495	3502	3514	rBV2	1822511	3559684	93.88%	6.703%
38	23.839	3521	3528	3540	rVB	1148452	2277891	60.08%	4.289%




Sum of corrected areas: 53106700

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029649.D
Acq On : 10 Feb 2024 15:48
Operator : MA/JU
Sample : PB158929BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK929

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

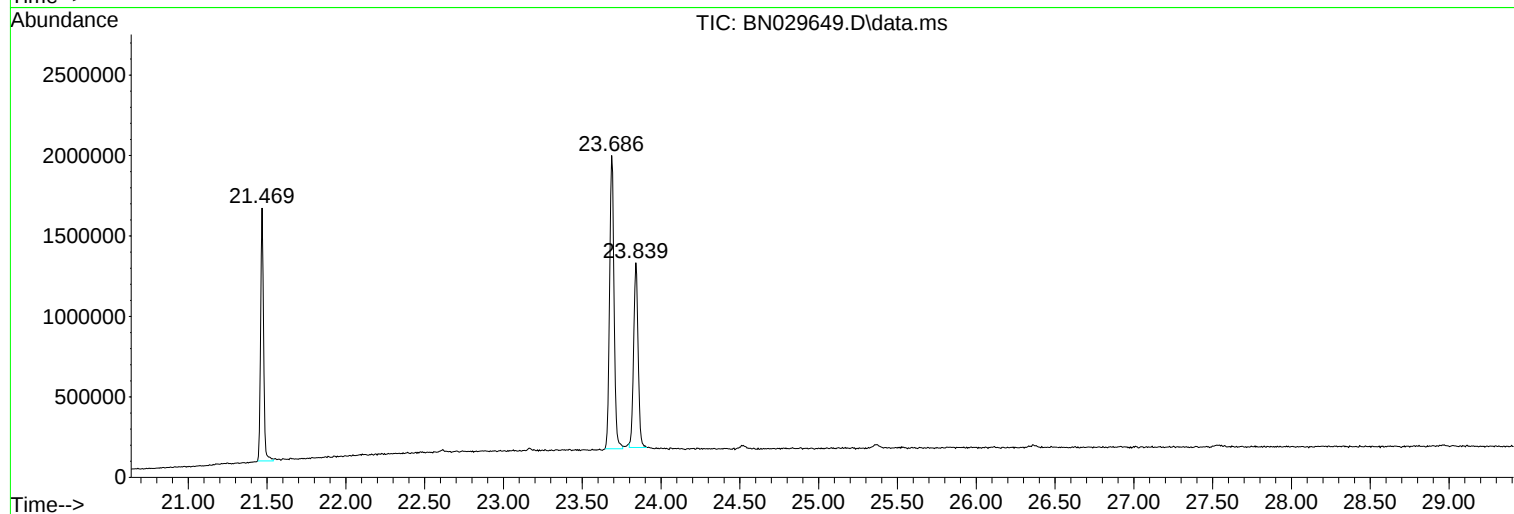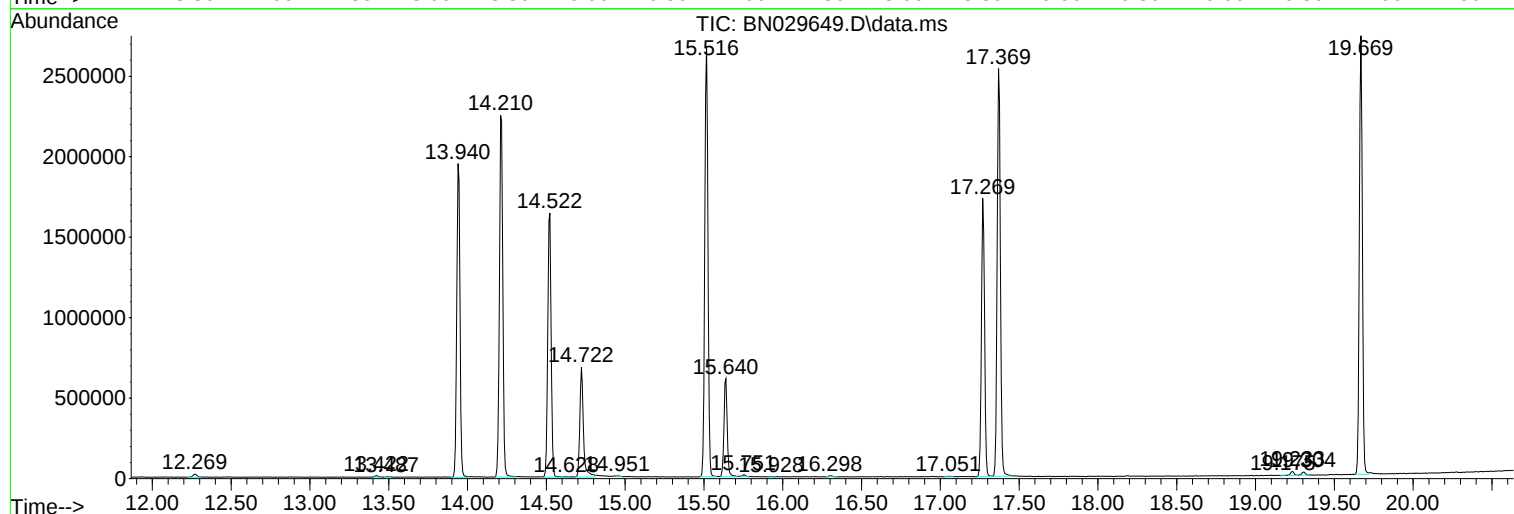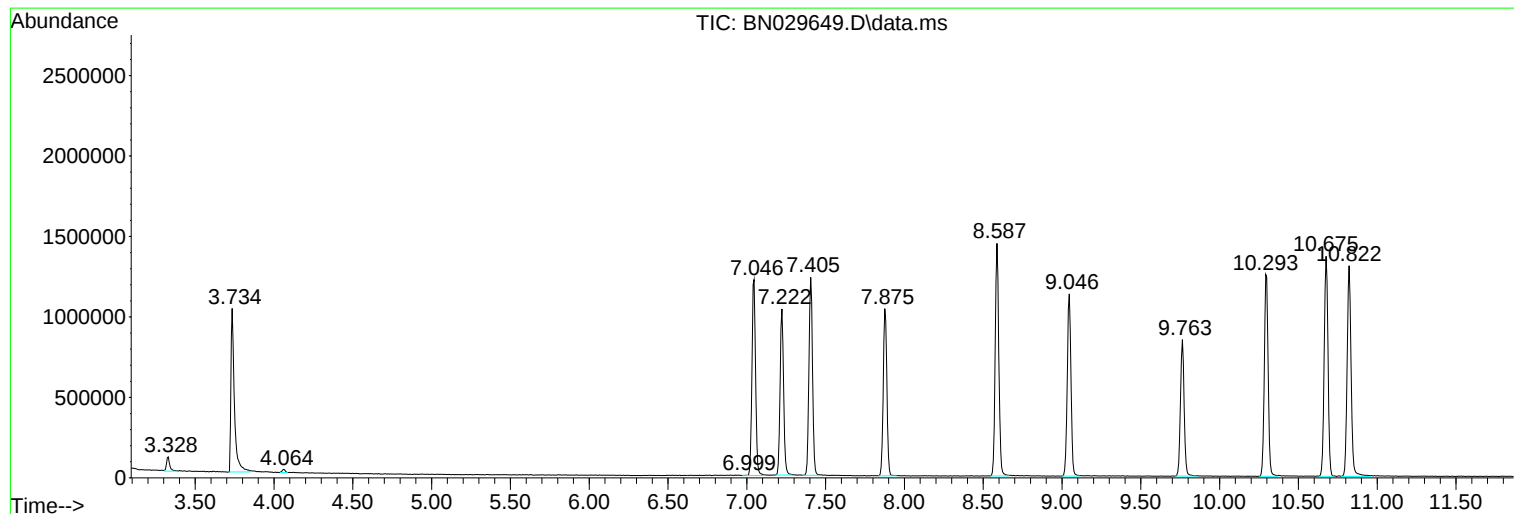

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029649.D
Acq On : 10 Feb 2024 15:48
Operator : MA/JU
Sample : PB158929BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK929

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029649.D
Acq On : 10 Feb 2024 15:48
Operator : MA/JU
Sample : PB158929BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK929

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------