

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029651.D
 Acq On : 10 Feb 2024 17:00
 Operator : MA/JU
 Sample : P1399-09
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	49	rVB	62225	83046	1.71%	0.148%
2	3.740	107	111	122	rBV	348333	591361	12.15%	1.057%
3	4.064	162	166	173	rVB	18439	26500	0.54%	0.047%
4	6.963	654	659	663	rVB6	4256	5981	0.12%	0.011%
5	7.040	666	672	685	rVB	364696	591625	12.16%	1.058%
6	7.222	696	703	715	rBV	1263613	1962980	40.33%	3.509%
7	7.405	726	734	745	rBV	1208054	1901435	39.07%	3.399%
8	7.493	746	749	752	rVB4	4336	5814	0.12%	0.010%
9	7.875	806	814	821	rBV	905731	1442208	29.63%	2.578%
10	8.587	928	935	946	rBV	960491	1523998	31.31%	2.724%
11	9.046	1005	1013	1022	rBV	1429499	2307431	47.41%	4.124%
12	9.210	1038	1041	1045	rVB4	3673	4998	0.10%	0.009%
13	9.434	1076	1079	1084	rVB3	4025	5881	0.12%	0.011%
14	9.763	1126	1135	1148	rBV	1047115	1697229	34.87%	3.034%
15	10.293	1218	1225	1243	rBV	1456135	2474130	50.83%	4.422%
16	10.675	1282	1290	1296	rBV	1211721	2025599	41.62%	3.621%
17	10.722	1296	1298	1305	rVB	23904	36075	0.74%	0.064%
18	10.822	1307	1315	1332	rBV	1383875	2393308	49.17%	4.278%
19	12.269	1556	1561	1569	rBV	24184	41116	0.84%	0.073%
20	12.881	1661	1665	1668	rBV4	3756	4987	0.10%	0.009%
21	13.351	1741	1745	1750	rVB7	3689	6260	0.13%	0.011%
22	13.422	1753	1757	1764	rBV2	22092	34993	0.72%	0.063%
23	13.945	1839	1846	1862	rBV	2430140	3501802	71.94%	6.259%
24	14.216	1883	1892	1904	rBV	2848047	4284471	88.02%	7.658%
25	14.522	1936	1944	1952	rBV	1471088	2217164	45.55%	3.963%
26	14.722	1973	1978	1989	rBV	138937	251692	5.17%	0.450%
27	14.940	2011	2015	2018	rBV6	3947	6020	0.12%	0.011%
28	15.516	2106	2113	2127	rBV	3414106	4867338	100.00%	8.700%
29	15.639	2127	2134	2144	rBV	879178	1230254	25.28%	2.199%
30	15.757	2150	2154	2160	rVB4	16954	26547	0.55%	0.047%
31	15.992	2190	2194	2199	rBV4	6579	9081	0.19%	0.016%
32	16.304	2242	2247	2253	rBV8	9077	13527	0.28%	0.024%
33	16.745	2318	2322	2328	rBV3	15184	18828	0.39%	0.034%
34	16.875	2338	2344	2349	rVB7	2585	5903	0.12%	0.011%
35	17.051	2372	2374	2381	rVB7	3611	6132	0.13%	0.011%
36	17.269	2405	2411	2420	rBV	1494622	2124931	43.66%	3.798%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029651.D
 Acq On : 10 Feb 2024 17:00
 Operator : MA/JU
 Sample : P1399-09
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	17.369	2422	2428	2441	rVV2	3214271	4747619	97.54%	8.486%
38	17.575	2457	2463	2467	rBV2	12931	18640	0.38%	0.033%
39	17.669	2476	2479	2483	rBV5	5590	8430	0.17%	0.015%
40	17.828	2501	2506	2509	rBV6	2892	5082	0.10%	0.009%
41	18.181	2561	2566	2573	rBV2	47824	68857	1.41%	0.123%
42	18.622	2636	2641	2644	rBV4	12091	15977	0.33%	0.029%
43	19.228	2740	2744	2752	rBV4	32764	52073	1.07%	0.093%
44	19.304	2752	2757	2761	rVV	31442	46008	0.95%	0.082%
45	19.345	2761	2764	2767	rVV5	8982	12550	0.26%	0.022%
46	19.375	2767	2769	2775	rVB7	5580	9925	0.20%	0.018%
47	19.463	2781	2784	2790	rBV7	17613	25591	0.53%	0.046%
48	19.628	2808	2812	2813	rBV4	6604	7160	0.15%	0.013%
49	19.669	2813	2819	2827	rVV	3547404	4756662	97.73%	8.502%
50	21.198	3076	3079	3085	rBV6	28860	41861	0.86%	0.075%
51	21.469	3120	3125	3138	rBV	1363154	1772127	36.41%	3.168%
52	23.692	3495	3503	3515	rBV2	2345632	4680171	96.15%	8.366%
53	23.839	3522	3528	3540	rVB	950554	1945670	39.97%	3.478%




Sum of corrected areas: 55945048

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029651.D
Acq On : 10 Feb 2024 17:00
Operator : MA/JU
Sample : P1399-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

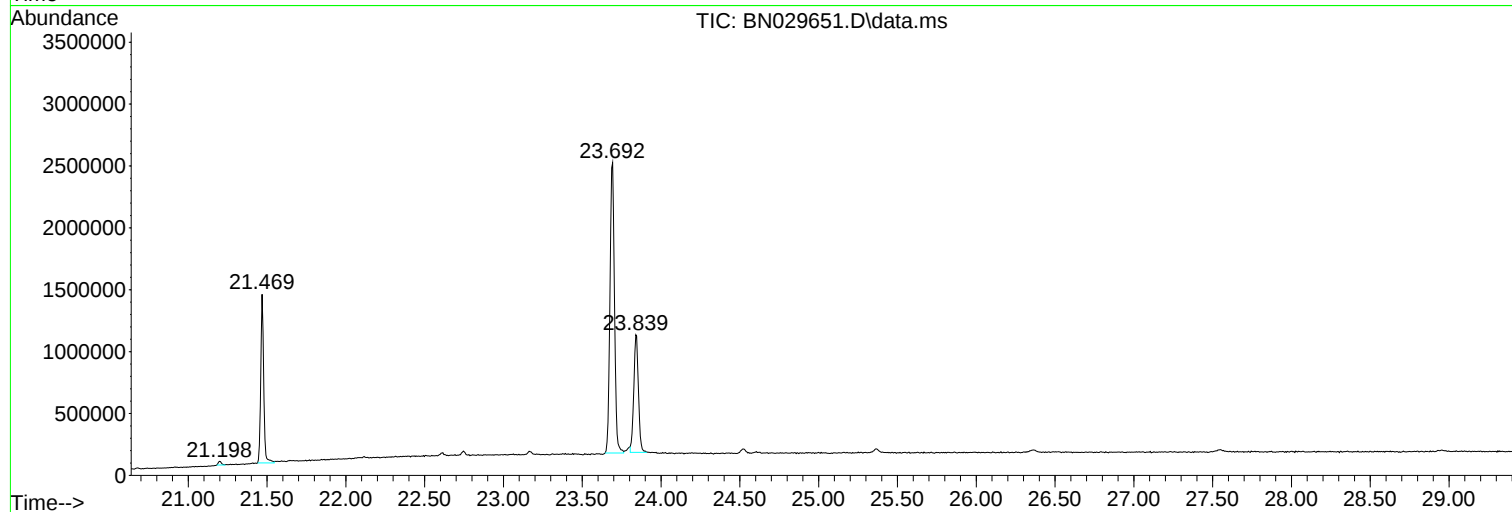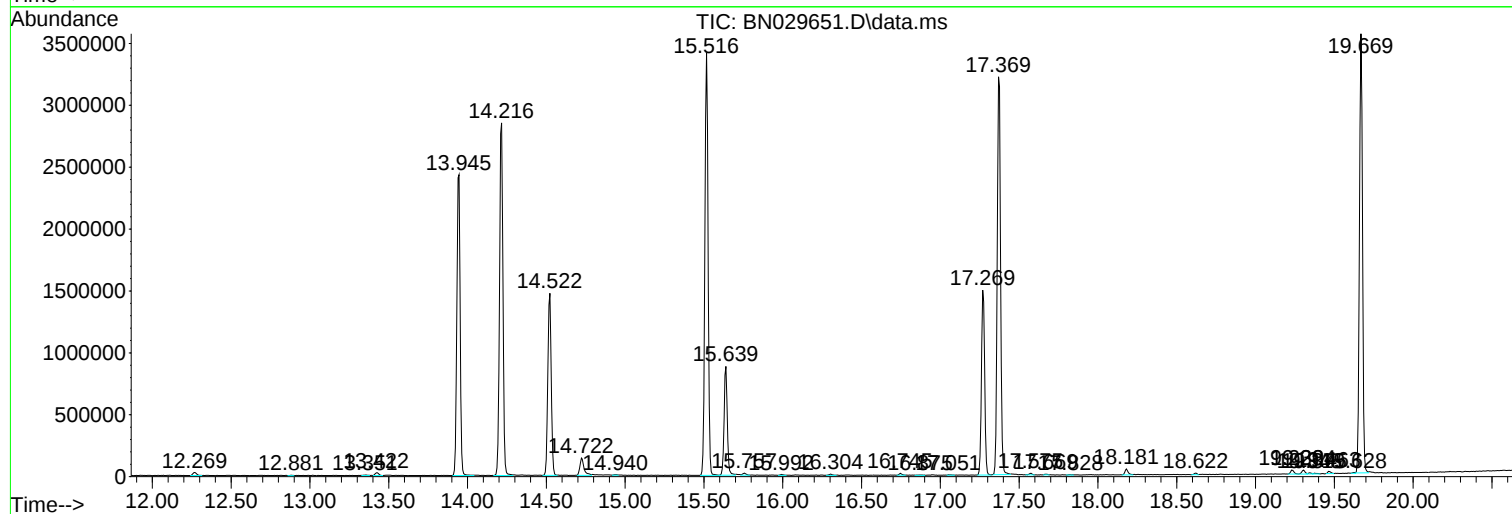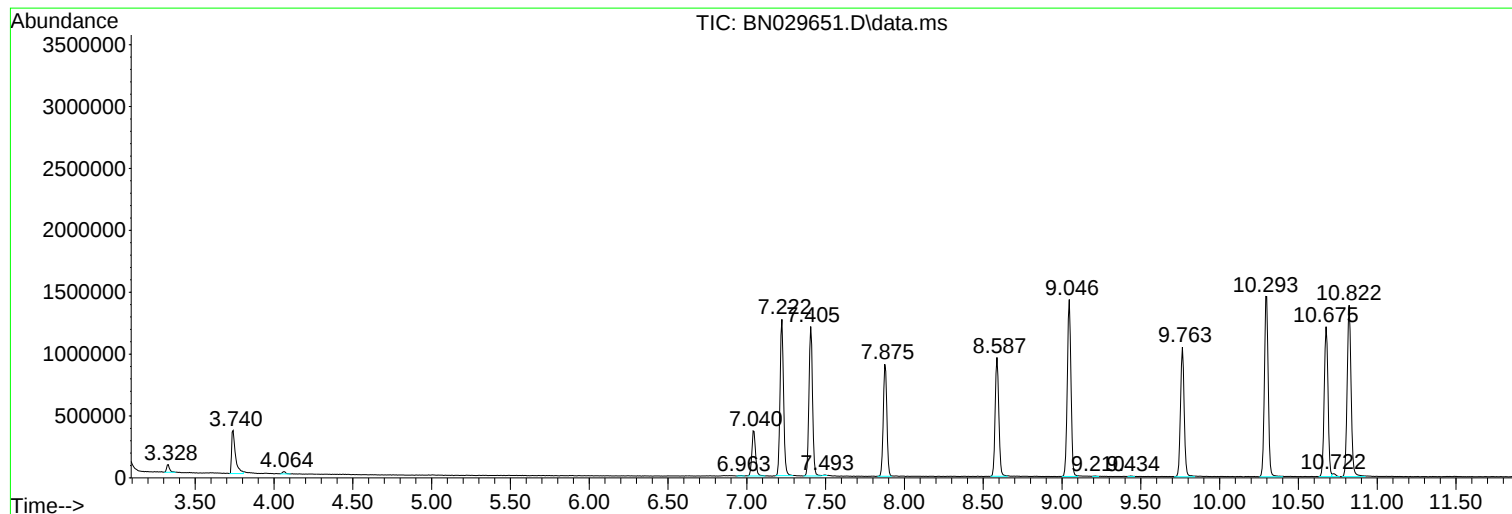

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029651.D
Acq On : 10 Feb 2024 17:00
Operator : MA/JU
Sample : P1399-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029651.D
Acq On : 10 Feb 2024 17:00
Operator : MA/JU
Sample : P1399-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------