

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029652.D
 Acq On : 10 Feb 2024 17:36
 Operator : MA/JU
 Sample : P1399-10
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	50	rVB	63985	89639	1.94%	0.170%
2	3.740	109	111	125	rBV	148369	278740	6.04%	0.527%
3	4.064	162	166	171	rVB	18624	24998	0.54%	0.047%
4	5.011	323	327	333	rVB8	5269	9087	0.20%	0.017%
5	5.158	349	352	358	rVB7	6830	8672	0.19%	0.016%
6	5.381	388	390	397	rVB8	3327	6524	0.14%	0.012%
7	5.887	472	476	480	rVB7	4159	6373	0.14%	0.012%
8	7.040	665	672	685	rVB	333682	563359	12.21%	1.066%
9	7.222	695	703	716	rBV	1260939	2000509	43.34%	3.784%
10	7.405	727	734	745	rBV	1224667	1896246	41.08%	3.587%
11	7.487	745	748	752	rBV6	6259	9127	0.20%	0.017%
12	7.875	807	814	822	rBV	876894	1392142	30.16%	2.634%
13	8.587	928	935	949	rBV	909552	1454285	31.51%	2.751%
14	9.046	1005	1013	1025	rBV	1384187	2295812	49.74%	4.343%
15	9.152	1026	1031	1037	rVV3	20429	39618	0.86%	0.075%
16	9.210	1039	1041	1046	rVB5	4307	5352	0.12%	0.010%
17	9.440	1076	1080	1086	rVB9	3491	5710	0.12%	0.011%
18	9.763	1126	1135	1148	rBV	1032624	1672269	36.23%	3.164%
19	10.293	1217	1225	1234	rBV	1423899	2414816	52.32%	4.568%
20	10.675	1283	1290	1298	rBV	1130656	1900385	41.17%	3.595%
21	10.822	1307	1315	1330	rBV	1198319	2114968	45.82%	4.001%
22	11.499	1424	1430	1435	rBV8	8714	18861	0.41%	0.036%
23	12.110	1530	1534	1537	rBV5	3516	5519	0.12%	0.010%
24	12.269	1555	1561	1566	rBV2	23043	37187	0.81%	0.070%
25	13.346	1741	1744	1750	rBV7	4949	8576	0.19%	0.016%
26	13.422	1752	1757	1762	rBV3	18036	26475	0.57%	0.050%
27	13.940	1838	1845	1855	rBV	2333684	3291598	71.31%	6.227%
28	14.216	1884	1892	1906	rBV	2685713	4092368	88.66%	7.742%
29	14.434	1923	1929	1931	rBV5	7821	11756	0.25%	0.022%
30	14.522	1937	1944	1952	rVB	1344700	2026104	43.90%	3.833%
31	14.722	1972	1978	1990	rBV	115251	214928	4.66%	0.407%
32	15.381	2087	2090	2094	rBV5	6951	9011	0.20%	0.017%
33	15.516	2106	2113	2126	rBV	3232939	4615741	100.00%	8.732%
34	15.640	2127	2134	2142	rBV	766129	1089967	23.61%	2.062%
35	15.757	2149	2154	2159	rBV4	12890	19721	0.43%	0.037%
36	16.081	2202	2209	2210	rBV6	3665	4856	0.11%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
 Data File : BN029652.D
 Acq On : 10 Feb 2024 17:36
 Operator : MA/JU
 Sample : P1399-10
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	16.245	2234	2237	2242	rVV5	7086	8647	0.19%	0.016%
38	16.304	2242	2247	2251	rVB5	8888	12390	0.27%	0.023%
39	17.051	2368	2374	2377	rBV6	5200	8498	0.18%	0.016%
40	17.269	2405	2411	2421	rBV	1394892	1975792	42.81%	3.738%
41	17.369	2421	2428	2449	rVV2	3060014	4449441	96.40%	8.417%
42	17.675	2477	2480	2483	rVB5	5128	7255	0.16%	0.014%
43	17.781	2495	2498	2503	rBV5	5057	7224	0.16%	0.014%
44	18.181	2561	2566	2573	rBV4	17431	25724	0.56%	0.049%
45	18.486	2615	2618	2619	rBV3	4888	5744	0.12%	0.011%
46	19.233	2740	2745	2751	rBV3	33230	48221	1.04%	0.091%
47	19.304	2753	2757	2762	rBV2	26101	38875	0.84%	0.074%
48	19.469	2778	2785	2789	rBV6	15378	25406	0.55%	0.048%
49	19.622	2807	2811	2813	rBV4	7494	11367	0.25%	0.022%
50	19.669	2813	2819	2828	rVV	3301171	4490599	97.29%	8.495%
51	20.228	2912	2914	2917	rBV4	4915	6746	0.15%	0.013%
52	20.392	2940	2942	2944	rBV3	6065	6355	0.14%	0.012%
53	21.469	3120	3125	3137	rBV	1255955	1704772	36.93%	3.225%
54	23.692	3495	3503	3517	rBV2	2232171	4432208	96.02%	8.385%
55	23.845	3522	3529	3542	rVB	922865	1934310	41.91%	3.659%




Sum of corrected areas: 52860873

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029652.D
Acq On : 10 Feb 2024 17:36
Operator : MA/JU
Sample : P1399-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

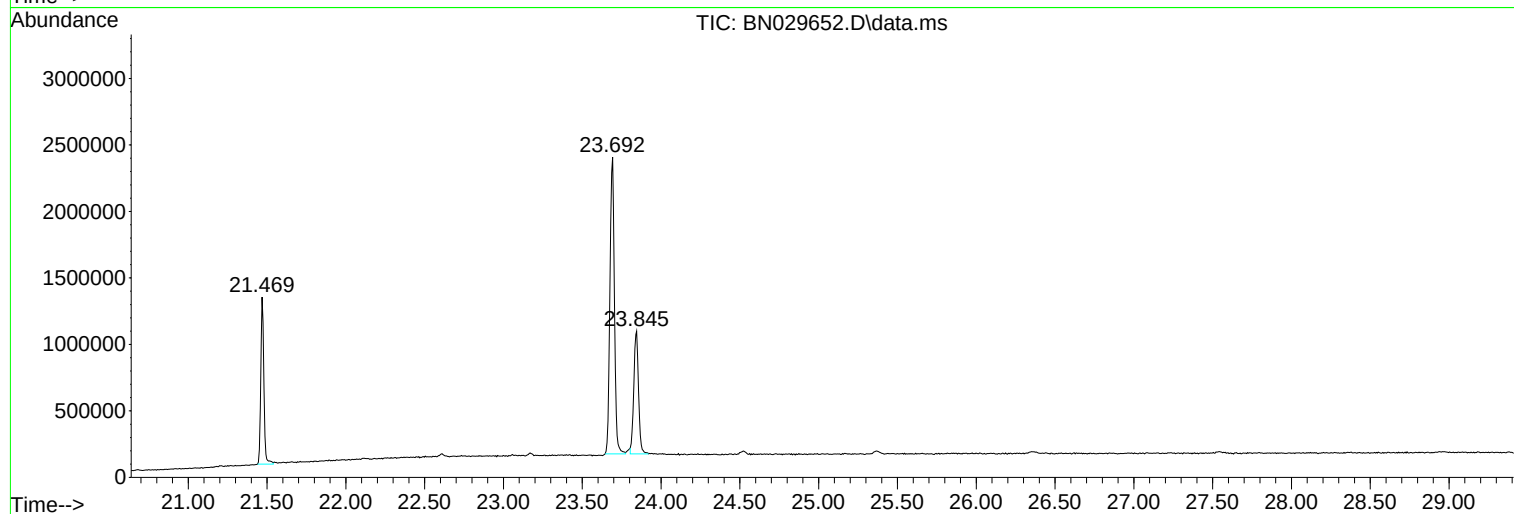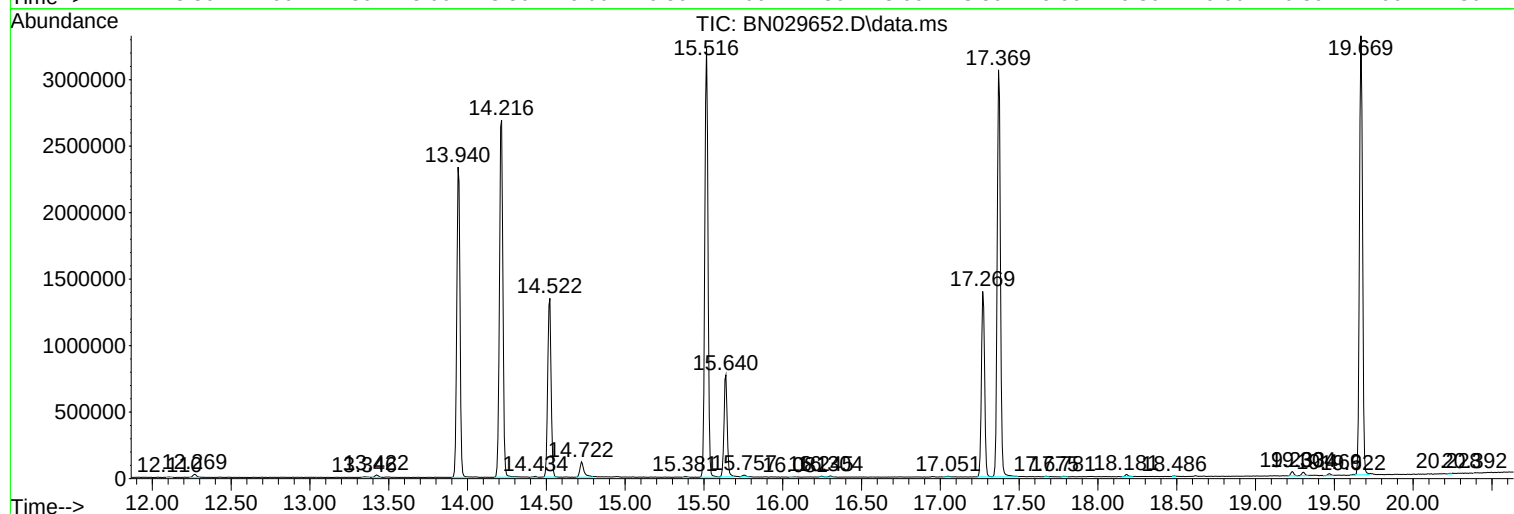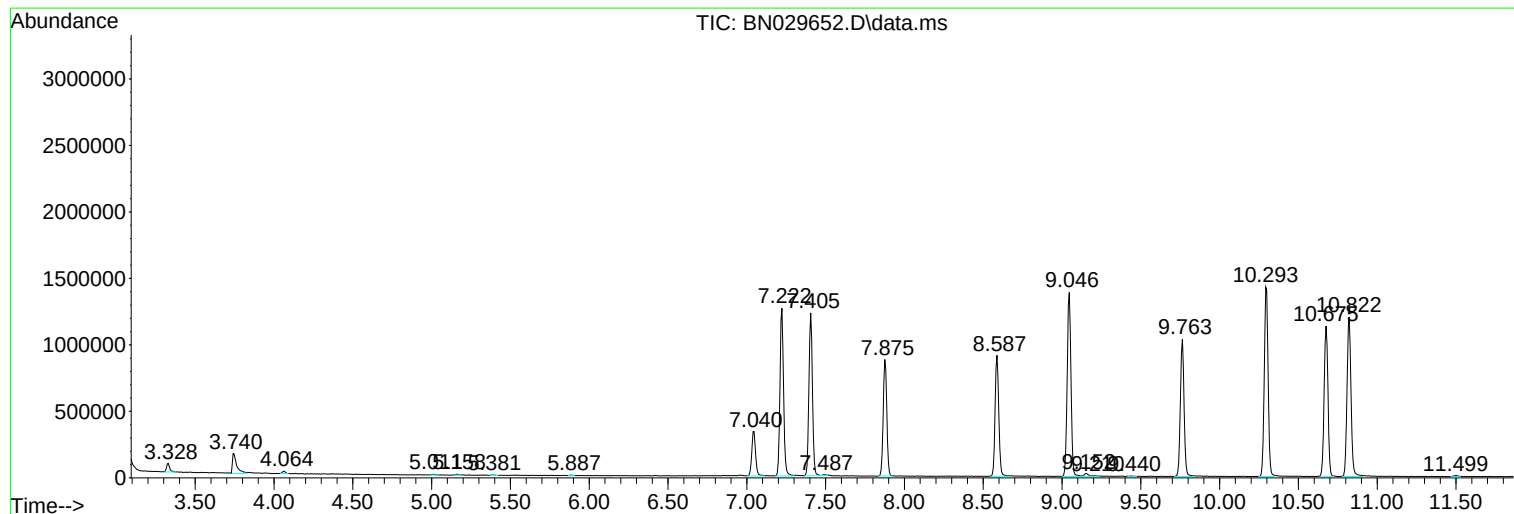

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029652.D
Acq On : 10 Feb 2024 17:36
Operator : MA/JU
Sample : P1399-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020924\
Data File : BN029652.D
Acq On : 10 Feb 2024 17:36
Operator : MA/JU
Sample : P1399-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------