

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021023\
 Data File : BN024001.D
 Acq On : 10 Feb 2023 11:13
 Operator : CG/JU
 Sample : PB150762BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK762

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
 Title : SVOA CALIBRATION

Signal : TIC: BN024001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	30	rBV	46238	60627	1.38%	0.128%
2	3.652	92	96	114	rBV	534102	863885	19.70%	1.822%
3	3.975	148	151	156	rVB	12562	16752	0.38%	0.035%
4	6.999	659	665	675	rBV	751136	1157493	26.39%	2.442%
5	7.169	687	694	706	rVB	612314	937808	21.38%	1.978%
6	7.364	720	727	741	rBV	764488	1203453	27.44%	2.539%
7	7.834	798	807	819	rBV	732493	1177382	26.85%	2.484%
8	8.552	922	929	939	rBV	907702	1412437	32.21%	2.979%
9	9.005	998	1006	1017	rBV	724965	1159912	26.45%	2.447%
10	9.722	1121	1128	1137	rBV	630365	995654	22.70%	2.100%
11	10.263	1213	1220	1230	rBV	956652	1505031	34.32%	3.175%
12	10.640	1277	1284	1296	rVB	1071480	1713324	39.07%	3.614%
13	10.787	1302	1309	1326	rBV	882595	1503720	34.29%	3.172%
14	12.234	1549	1555	1561	rVB3	13808	23283	0.53%	0.049%
15	13.381	1745	1750	1759	rVV3	12643	19774	0.45%	0.042%
16	13.904	1829	1839	1849	rBV	1669493	2234006	50.94%	4.712%
17	14.181	1879	1886	1904	rBV	1889602	2577104	58.76%	5.436%
18	14.487	1931	1938	1951	rBV	1673638	2316723	52.82%	4.887%
19	14.693	1967	1973	1992	rBV	751777	1137837	25.94%	2.400%
20	15.481	2097	2107	2122	rBV	2383287	3277445	74.73%	6.913%
21	15.604	2122	2128	2139	rVV	870727	1135114	25.88%	2.394%
22	15.722	2143	2148	2153	rVB4	9769	14422	0.33%	0.030%
23	17.022	2365	2369	2373	rBV3	3447	5035	0.11%	0.011%
24	17.239	2399	2406	2416	rBV	2111057	2889161	65.88%	6.094%
25	17.339	2416	2423	2440	rVV	2674903	3640691	83.01%	7.680%
26	19.198	2734	2739	2744	rBV2	31191	40393	0.92%	0.085%
27	19.269	2746	2751	2755	rBV	29411	40669	0.93%	0.086%
28	19.633	2807	2813	2822	rBV	3420652	4385681	100.00%	9.251%
29	21.427	3113	3118	3125	rBV	2605553	3086782	70.38%	6.511%
30	23.657	3489	3497	3507	rBV2	2006152	3952395	90.12%	8.337%
31	23.810	3516	3523	3535	rVB2	1596887	2922803	66.64%	6.165%




Sum of corrected areas: 47406796

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021023\
Data File : BN024001.D
Acq On : 10 Feb 2023 11:13
Operator : CG/JU
Sample : PB150762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK762

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

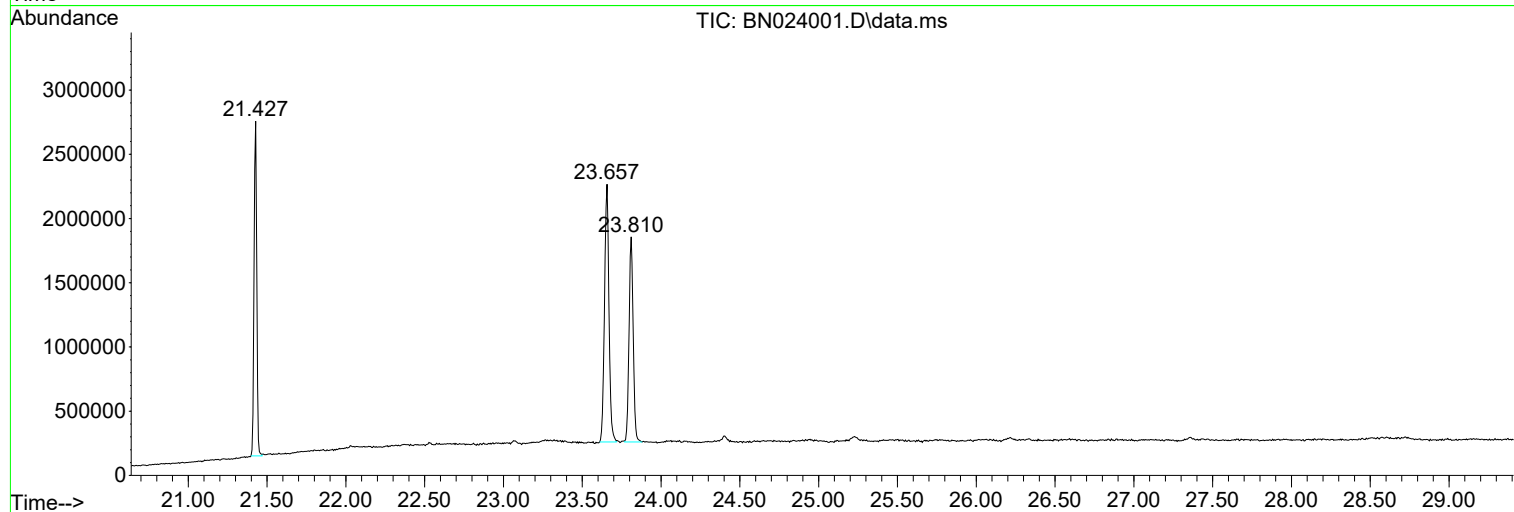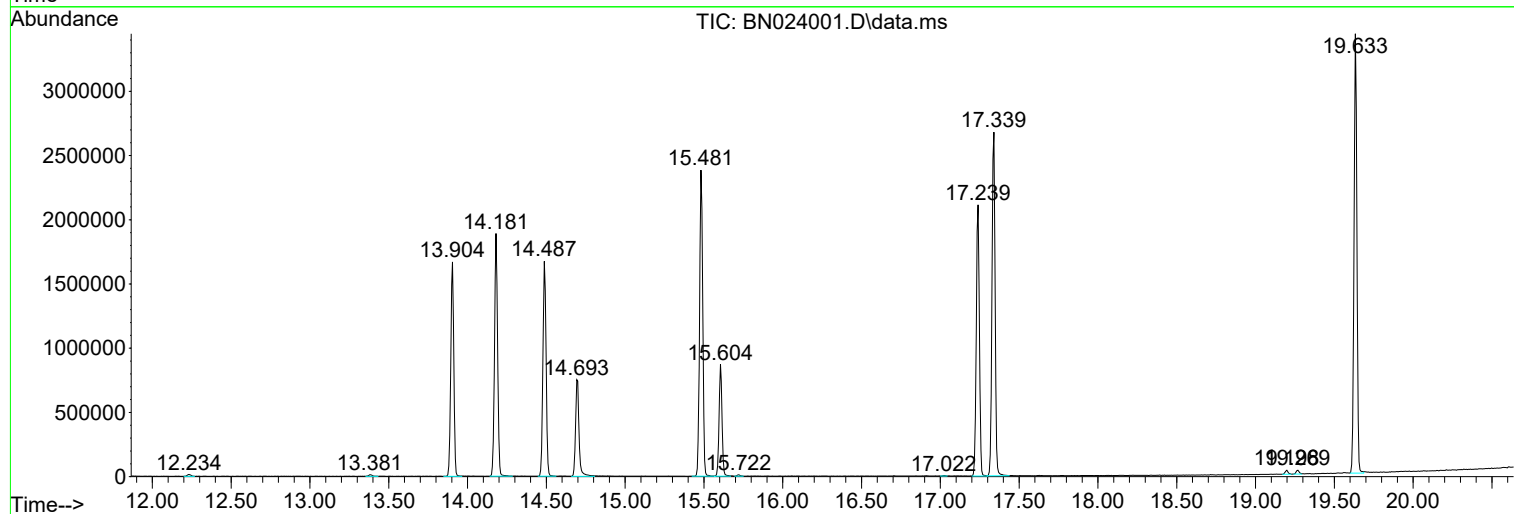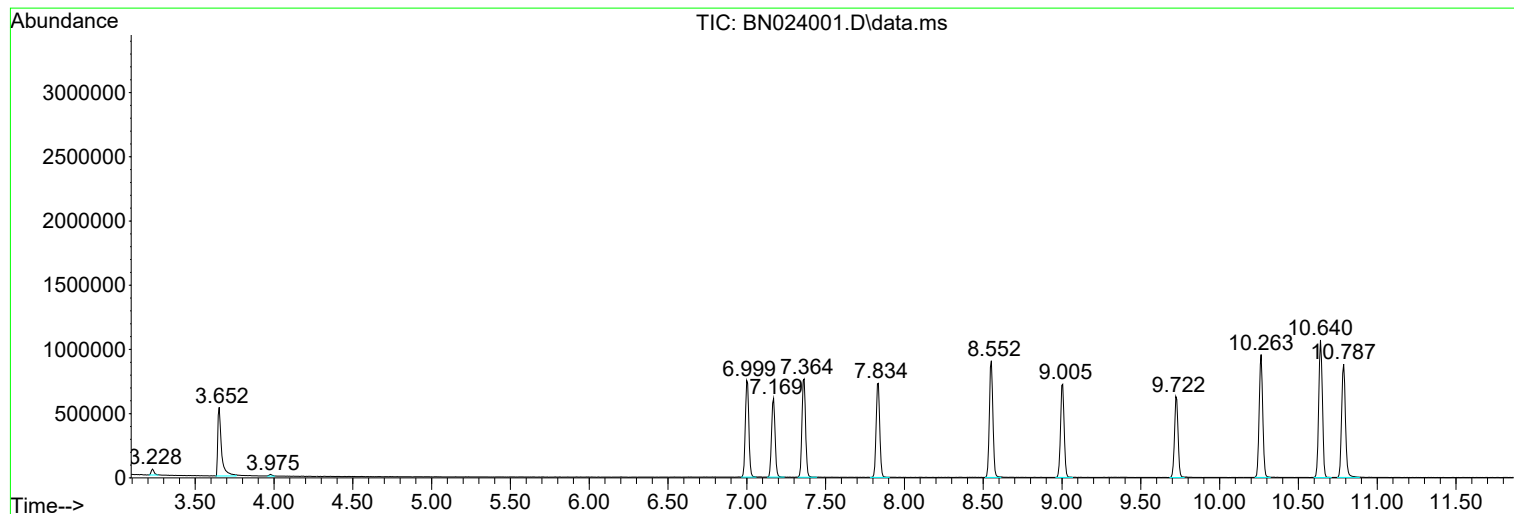

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021023\
Data File : BN024001.D
Acq On : 10 Feb 2023 11:13
Operator : CG/JU
Sample : PB150762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK762

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021023\
Data File : BN024001.D
Acq On : 10 Feb 2023 11:13
Operator : CG/JU
Sample : PB150762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK762

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc