

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021025\
 Data File : BN036411.D
 Acq On : 10 Feb 2025 13:36
 Operator : RC/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Feb 11 00:35:50 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 11 00:33:05 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.753	152	2219	0.400	ng	0.00
7) Naphthalene-d8	10.541	136	5528	0.400	ng	0.00
13) Acenaphthene-d10	14.388	164	3606	0.400	ng	0.00
19) Phenanthrene-d10	17.136	188	8328	0.400	ng	0.00
29) Chrysene-d12	21.322	240	7484	0.400	ng	0.00
35) Perylene-d12	23.595	264	7735	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.348	112	2078	0.368	ng	0.00
5) Phenol-d6	6.937	99	2290	0.348	ng	0.00
8) Nitrobenzene-d5	8.907	82	2015	0.391	ng	0.00
11) 2-Methylnaphthalene-d10	12.141	152	3329	0.440	ng	0.00
14) 2,4,6-Tribromophenol	15.882	330	670	0.302	ng	0.00
15) 2-Fluorobiphenyl	13.019	172	4965	0.323	ng	0.00
27) Fluoranthene-d10	19.169	212	8851	0.413	ng	0.00
31) Terphenyl-d14	19.768	244	6378	0.412	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.268	88	961	0.392	ng	99
3) n-Nitrosodimethylamine	3.579	42	1695	0.385	ng	100
6) bis(2-Chloroethyl)ether	7.183	93	2410	0.440	ng	100
9) Naphthalene	10.594	128	6168	0.391	ng	100
10) Hexachlorobutadiene	10.883	225	1567	0.317	ng	# 100
12) 2-Methylnaphthalene	12.212	142	4078	0.411	ng	100
16) Acenaphthylene	14.110	152	6103	0.366	ng	100
17) Acenaphthene	14.452	154	4132	0.362	ng	100
18) Fluorene	15.446	166	5991	0.407	ng	99
20) 4,6-Dinitro-2-methylph...	15.523	198	572	0.307	ng	100
21) 4-Bromophenyl-phenylether	16.329	248	1920	0.337	ng	100
22) Hexachlorobenzene	16.453	284	2369	0.318	ng	100
23) Atrazine	16.615	200	1560	0.372	ng	100
24) Pentachlorophenol	16.801	266	1018	0.313	ng	99
25) Phenanthrene	17.173	178	9119	0.374	ng	100
26) Anthracene	17.273	178	8056	0.363	ng	100
28) Fluoranthene	19.201	202	11264	0.389	ng	100
30) Pyrene	19.564	202	11479	0.384	ng	100
32) Benzo(a)anthracene	21.313	228	9677	0.364	ng	100
33) Chrysene	21.358	228	10178	0.373	ng	100
34) Bis(2-ethylhexyl)phtha...	21.241	149	5815	0.392	ng	100
36) Indeno(1,2,3-cd)pyrene	25.899	276	10661	0.351	ng	100
37) Benzo(b)fluoranthene	22.911	252	9743	0.355	ng	100
38) Benzo(k)fluoranthene	22.958	252	10543	0.377	ng	100
39) Benzo(a)pyrene	23.499	252	8521	0.362	ng	100
40) Dibenzo(a,h)anthracene	25.917	278	8314	0.344	ng	100
41) Benzo(g,h,i)perylene	26.601	276	9701	0.366	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021025\
Data File : BN036411.D
Acq On : 10 Feb 2025 13:36
Operator : RC/JU
Sample : SSTDICC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.4


Quant Time: Feb 11 00:35:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 11 00:33:05 2025
Response via : Initial Calibration

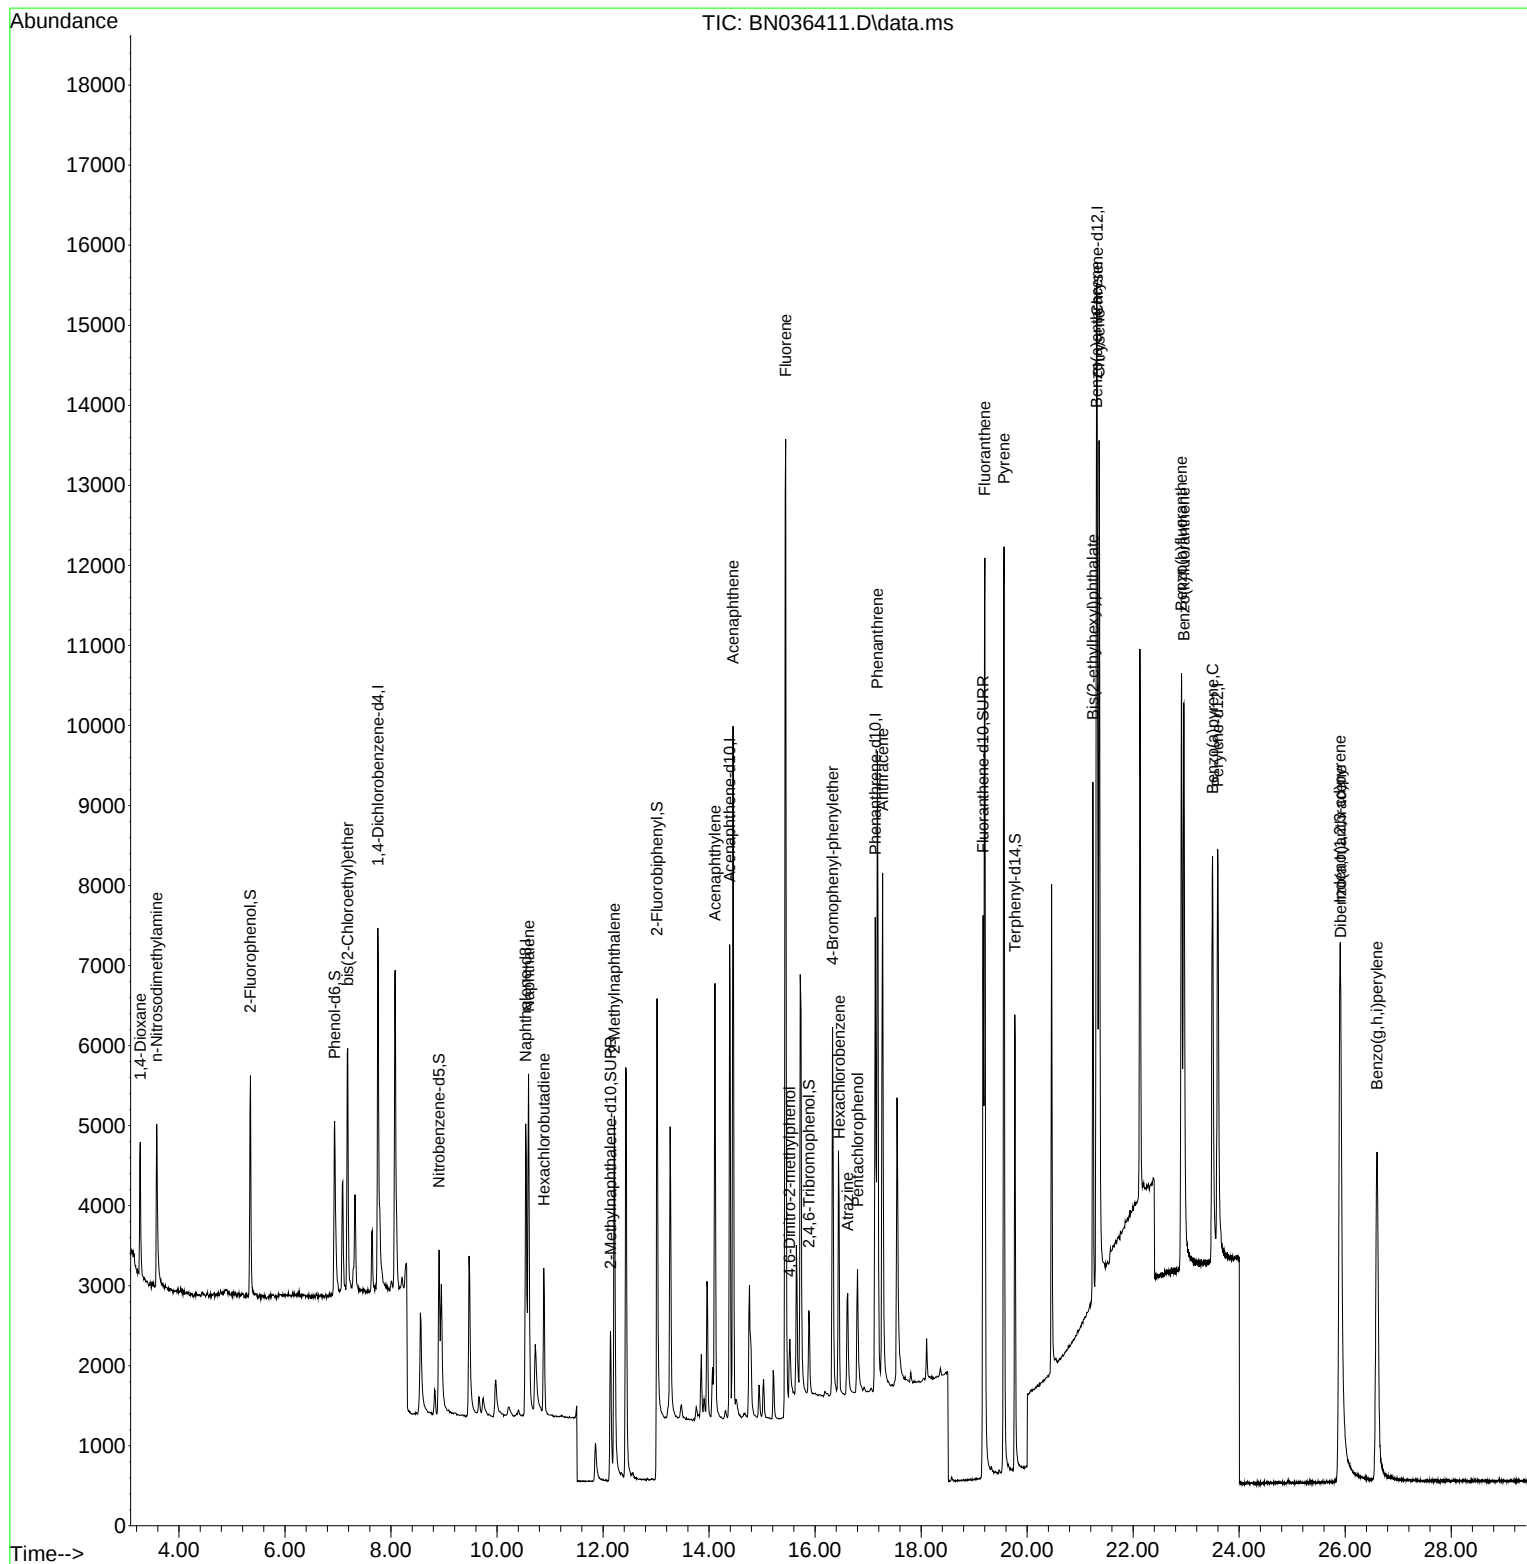





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.753 min Scan# 64
 Delta R.T. 0.000 min
 Lab File: BN036411.D
 Acq: 10 Feb 2025 13:36

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4







Tgt Ion:152 Resp: 2219
 Ion Ratio Lower Upper
 152 100
 150 154.6 123.7 185.5
 115 65.6 52.5 78.7

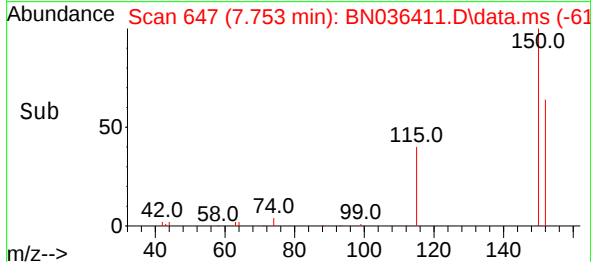

#2
 1,4-Dioxane
 Concen: 0.392 ng
 RT: 3.268 min Scan# 26
 Delta R.T. 0.000 min
 Lab File: BN036411.D
 Acq: 10 Feb 2025 13:36

Tgt Ion: 88 Resp: 961
 Ion Ratio Lower Upper
 88 100
 43 41.4 33.7 50.5
 58 87.1 68.9 103.3


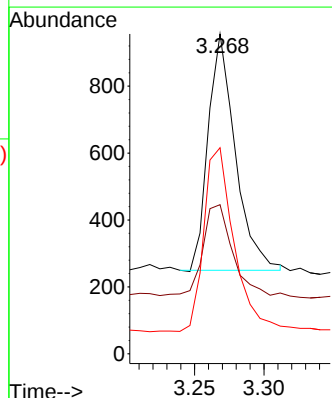
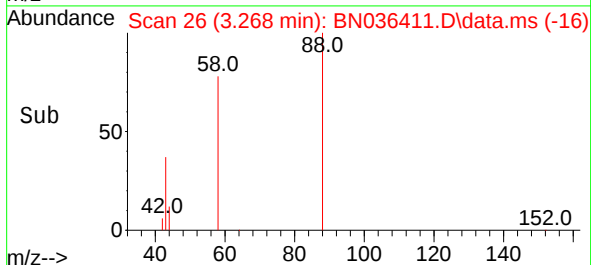
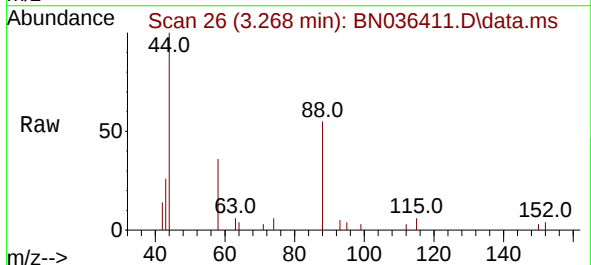


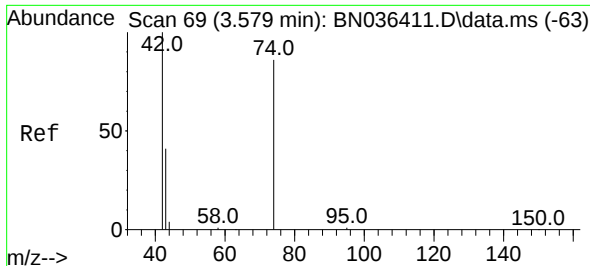

#3
n-Nitrosodimethylamine
Concen: 0.385 ng
RT: 3.579 min Scan# 69
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 42 Resp: 1695
Ion Ratio Lower Upper
42 100
74 89.7 71.8 107.6
44 9.7 7.8 11.6

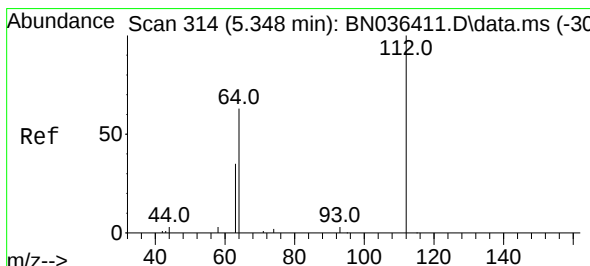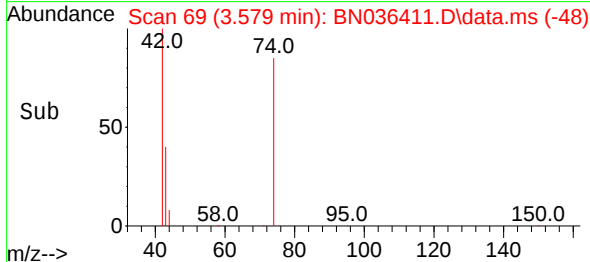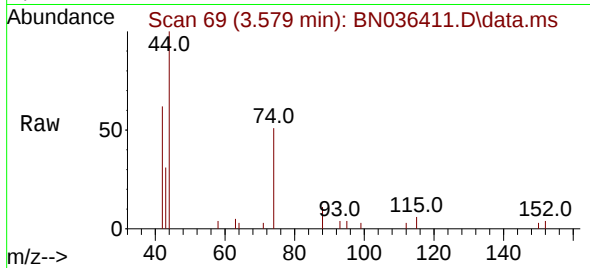

#4
2-Fluorophenol
Concen: 0.368 ng
RT: 5.348 min Scan# 314
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36

Tgt Ion: 112 Resp: 2078
Ion Ratio Lower Upper
112 100
64 66.7 53.4 80.0
63 37.9 30.3 45.5


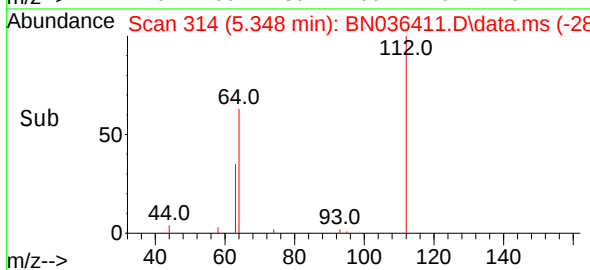

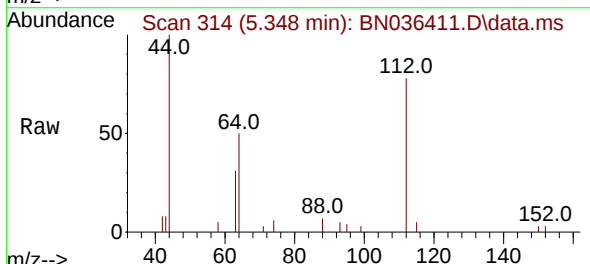




#5
Phenol-d6
Concen: 0.348 ng
RT: 6.937 min Scan# 534
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 99 Resp: 2290
Ion Ratio Lower Upper
99 100
42 27.1 21.7 32.5
71 40.8 32.6 49.0

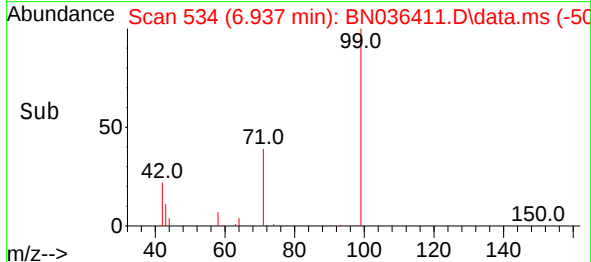

#6
bis(2-Chloroethyl)ether
Concen: 0.440 ng
RT: 7.183 min Scan# 568
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36

Tgt Ion: 93 Resp: 2410
Ion Ratio Lower Upper
93 100
63 82.9 66.3 99.5
95 32.8 26.2 39.4


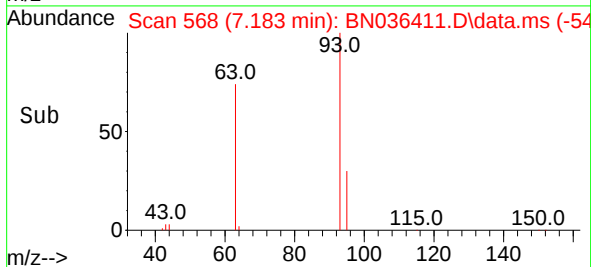

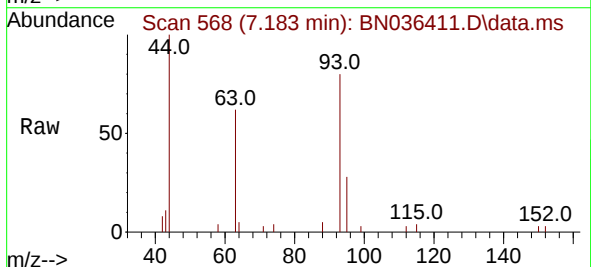




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.541 min Scan# 933
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	136	Resp:	5528
Ion	Ratio	Lower	Upper
136	100		
137	12.6	10.1	15.1
54	14.7	11.8	17.6
68	9.0	7.2	10.8

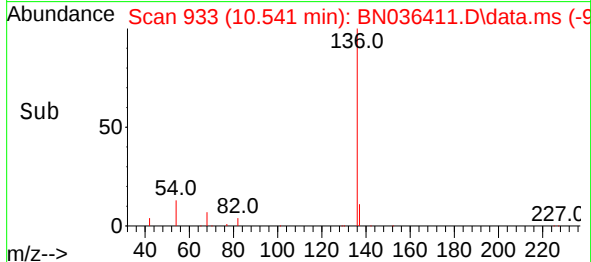

#8
Nitrobenzene-d5
Concen: 0.391 ng
RT: 8.907 min Scan# 780
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36

Tgt Ion:	82	Resp:	2015
Ion	Ratio	Lower	Upper
82	100		
128	39.9	31.9	47.9
54	66.4	53.1	79.7

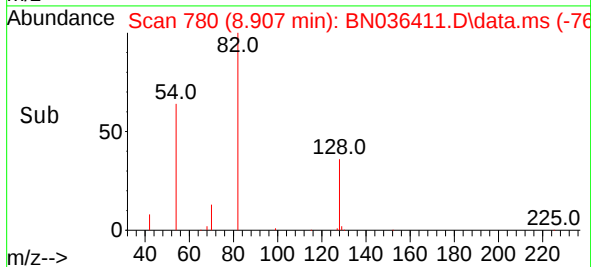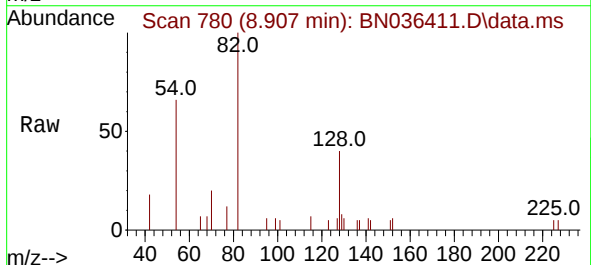



#9

Naphthalene

Concen: 0.391 ng

RT: 10.594 min Scan# 938

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:128 Resp: 6168

Ion Ratio Lower Upper

128 100

129 12.0 9.6 14.4

127 15.0 12.0 18.0

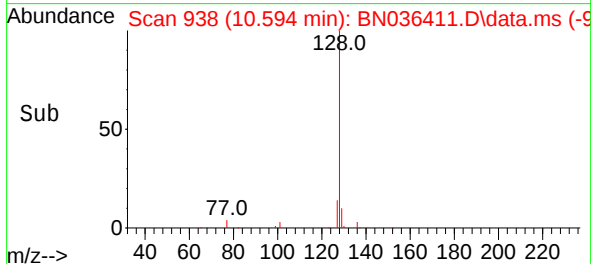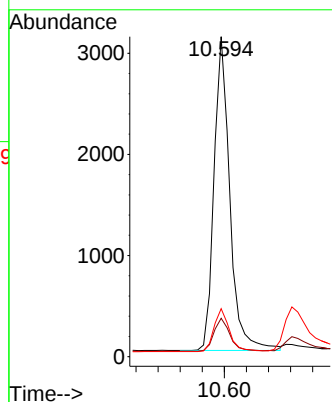

#10

Hexachlorobutadiene

Concen: 0.317 ng

RT: 10.883 min Scan# 965

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36




Tgt Ion:225 Resp: 1567


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.6 50.9 76.3


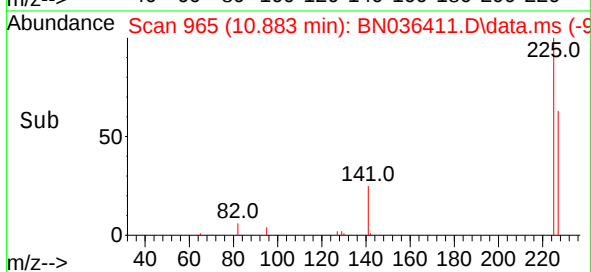
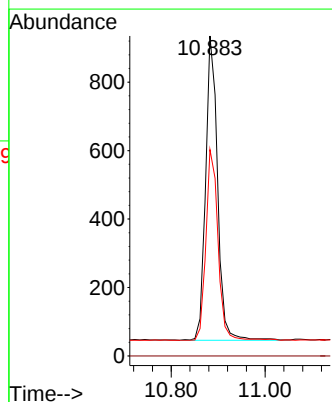





#11
2-Methylnaphthalene-d10
Concen: 0.440 ng
RT: 12.141 min Scan# 1148
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 3329
Ion Ratio Lower Upper
152 100
151 20.8 16.6 25.0

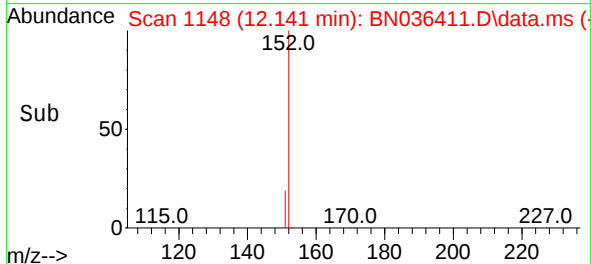

#12
2-Methylnaphthalene
Concen: 0.411 ng
RT: 12.212 min Scan# 1162
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36

Tgt Ion:142 Resp: 4078
Ion Ratio Lower Upper
142 100
141 91.0 72.8 109.2
115 44.4 35.5 53.3




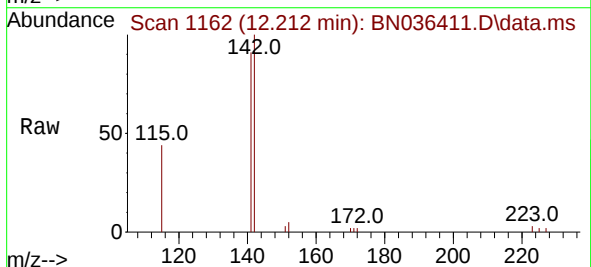




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.388 min Scan# 1448
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:164 Resp: 3606
Ion Ratio Lower Upper
164 100
162 105.1 84.1 126.1
160 51.7 41.4 62.0

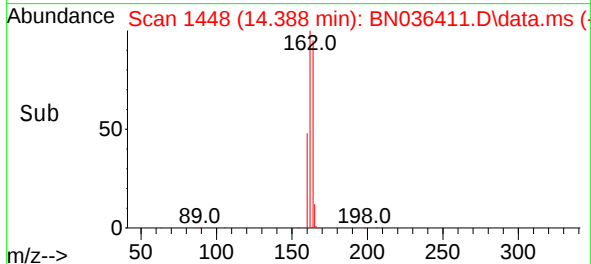

#14
2,4,6-Tribromophenol
Concen: 0.302 ng
RT: 15.882 min Scan# 1583
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36

Tgt Ion:330 Resp: 670
Ion Ratio Lower Upper
330 100
332 95.7 76.6 114.8
141 47.3 37.8 56.8




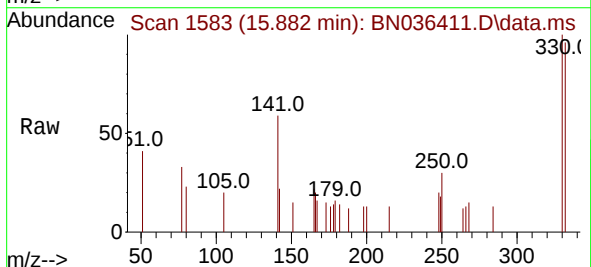


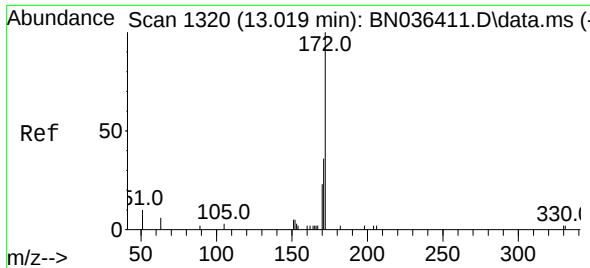

#15
2-Fluorobiphenyl
Concen: 0.323 ng
RT: 13.019 min Scan# 1320
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	172	Resp:	4965
Ion Ratio	Lower	Upper	
172	100		
171	37.0	29.6	44.4
170	24.7	19.8	29.6

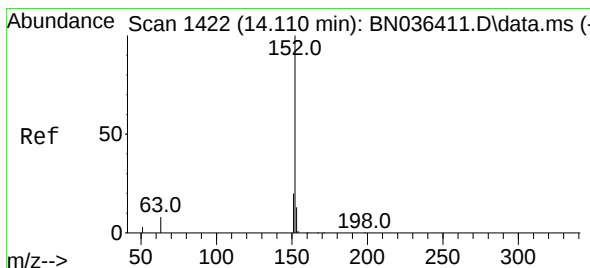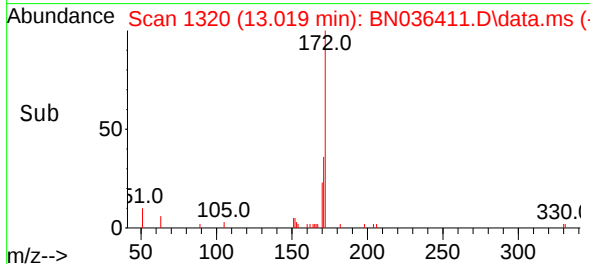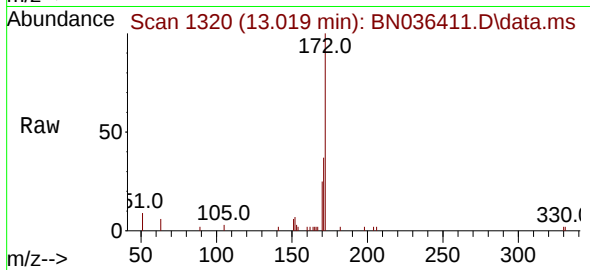

#16
Acenaphthylene
Concen: 0.366 ng
RT: 14.110 min Scan# 1422
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36

Tgt Ion:	152	Resp:	6103
Ion Ratio	Lower	Upper	
152	100		
151	19.8	15.8	23.8
153	12.7	10.2	15.2


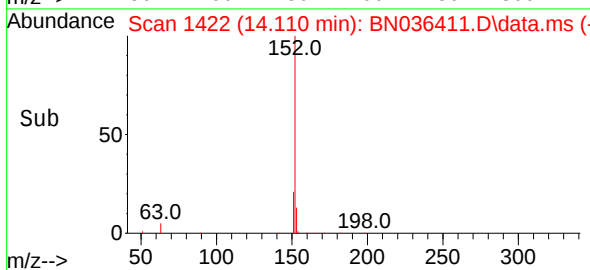

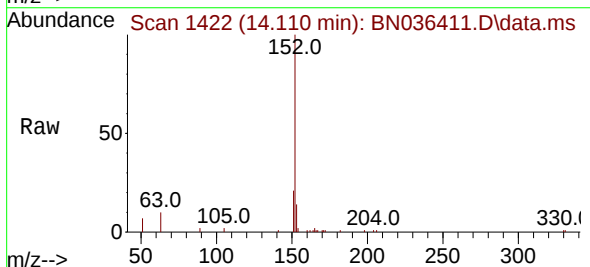


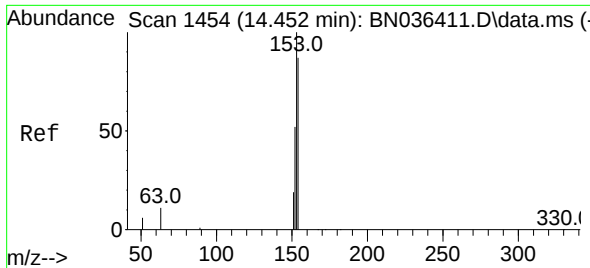

#17
Acenaphthene
Concen: 0.362 ng
RT: 14.452 min Scan# 1454
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:154 Resp: 4132
Ion Ratio Lower Upper
154 100
153 116.6 93.3 139.9
152 61.0 48.8 73.2

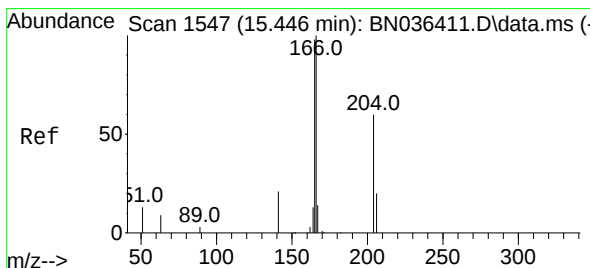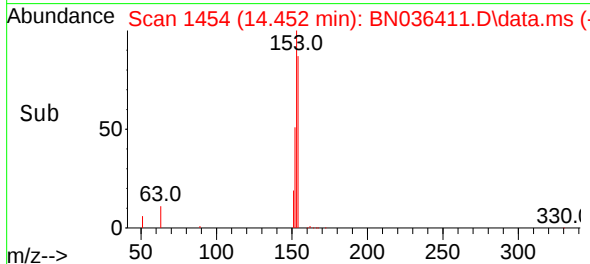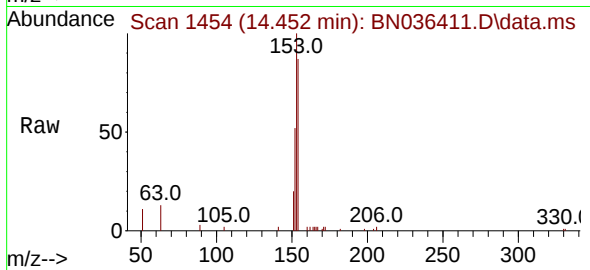

#18
Fluorene
Concen: 0.407 ng
RT: 15.446 min Scan# 1547
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36

Tgt Ion:166 Resp: 5991
Ion Ratio Lower Upper
166 100
165 100.0 79.5 119.3
167 13.0 10.4 15.6

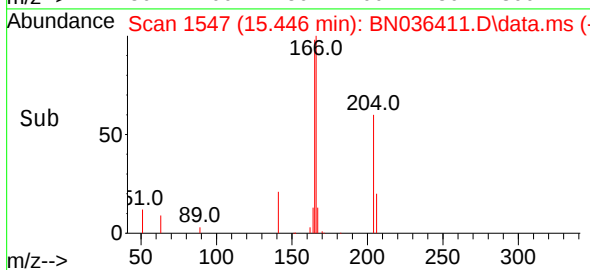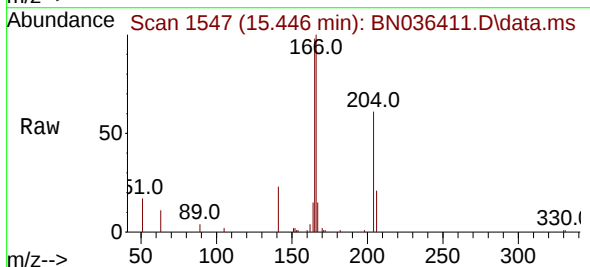



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.136 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:188 Resp: 8328

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 12.2 9.8 14.6

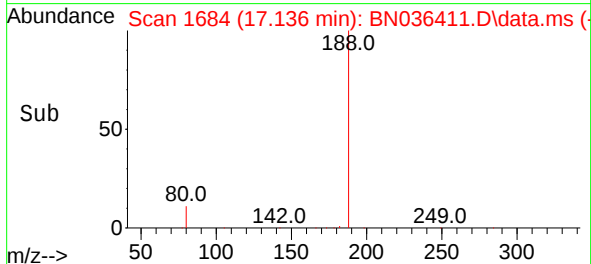

#20

4,6-Dinitro-2-methylphenol

Concen: 0.307 ng

RT: 15.523 min Scan# 1554

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36




Tgt Ion:198 Resp: 572


Ion Ratio Lower Upper

198 100

51 108.2 86.6 129.8

105 71.9 57.5 86.3




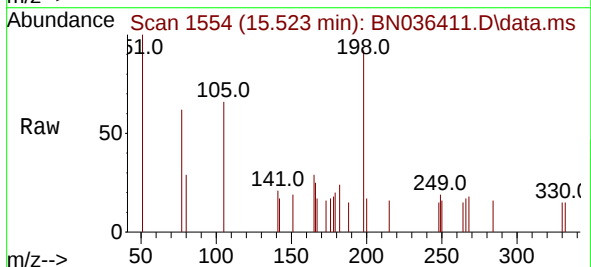




#21
4-Bromophenyl-phenylether
Concen: 0.337 ng
RT: 16.329 min Scan# 1619
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:248 Resp: 1920
Ion Ratio Lower Upper
248 100
250 95.1 76.1 114.1
141 89.6 71.7 107.5

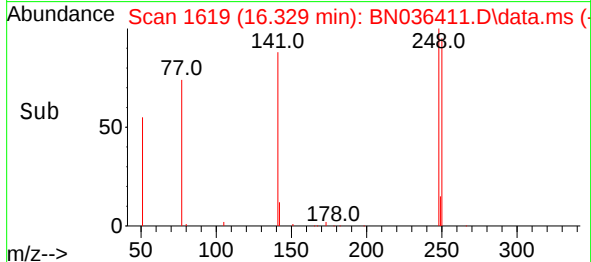

#22
Hexachlorobenzene
Concen: 0.318 ng
RT: 16.453 min Scan# 1629
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36

Tgt Ion:284 Resp: 2369
Ion Ratio Lower Upper
284 100
142 41.7 33.4 50.0
249 35.4 28.6 43.0


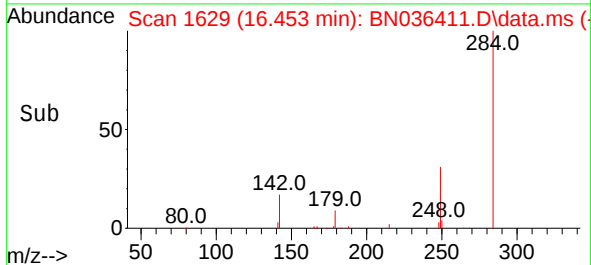

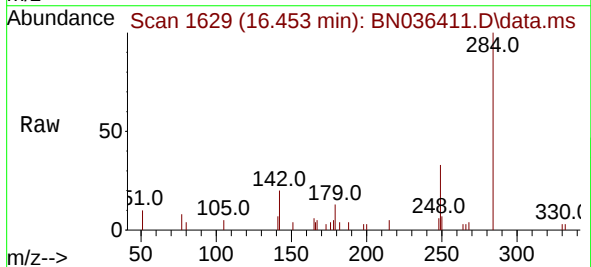




#23
 Atrazine
 Concen: 0.372 ng
 RT: 16.615 min Scan# 1642
 Delta R.T. 0.000 min
 Lab File: BN036411.D
 Acq: 10 Feb 2025 13:36




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4


Tgt Ion:200 Resp: 1560
 Ion Ratio Lower Upper
 200 100
 173 29.0 23.2 34.8
 215 50.0 40.0 60.0

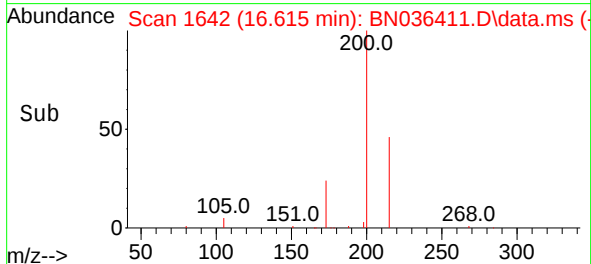

#24
 Pentachlorophenol
 Concen: 0.313 ng
 RT: 16.801 min Scan# 1657
 Delta R.T. 0.000 min
 Lab File: BN036411.D
 Acq: 10 Feb 2025 13:36

Tgt Ion:266 Resp: 1018
 Ion Ratio Lower Upper
 266 100
 264 64.0 50.6 76.0
 268 65.1 51.9 77.9




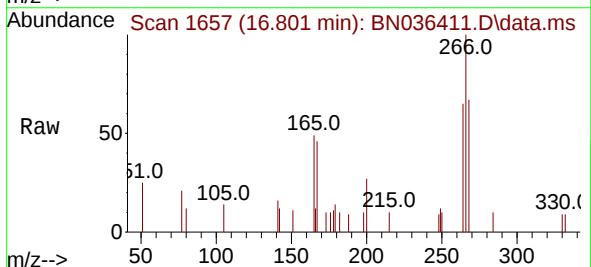


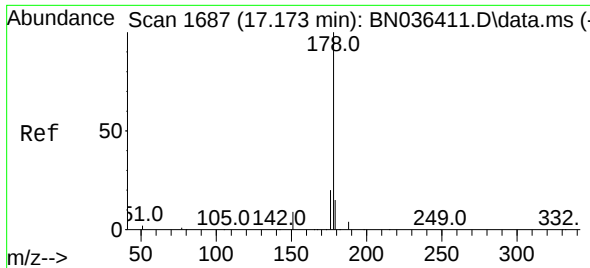

#25
Phenanthrene
Concen: 0.374 ng
RT: 17.173 min Scan# 1687
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:178 Resp: 9119
Ion Ratio Lower Upper
178 100
176 19.6 15.7 23.5
179 15.5 12.4 18.6

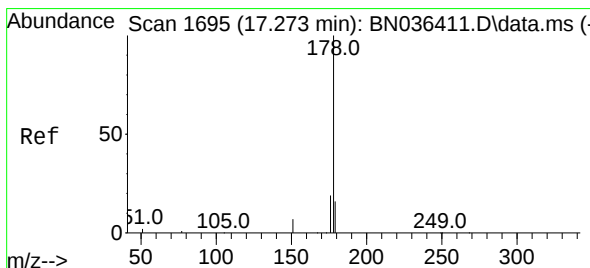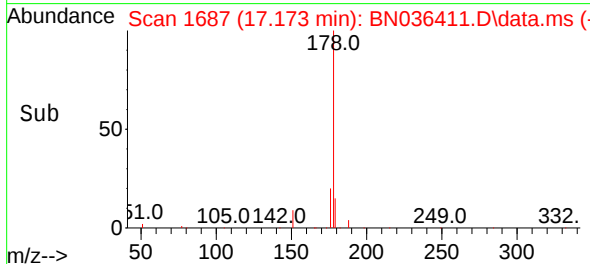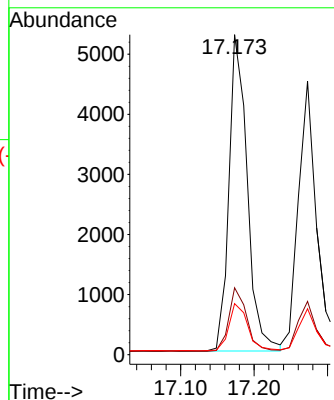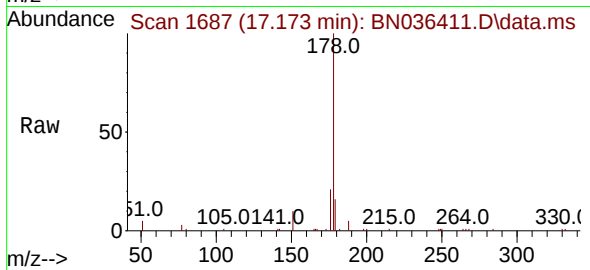

#26
Anthracene
Concen: 0.363 ng
RT: 17.273 min Scan# 1695
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36

Tgt Ion:178 Resp: 8056
Ion Ratio Lower Upper
178 100
176 18.7 14.9 22.3
179 15.3 12.4 18.6


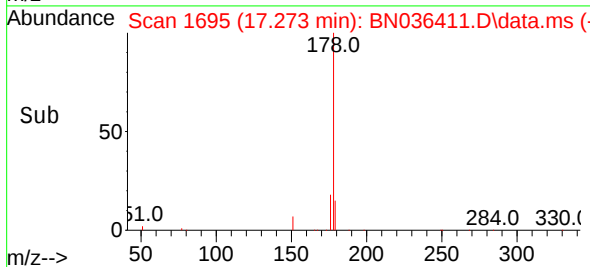
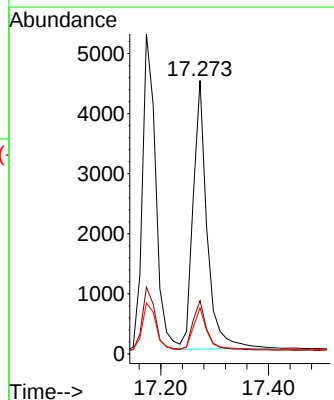
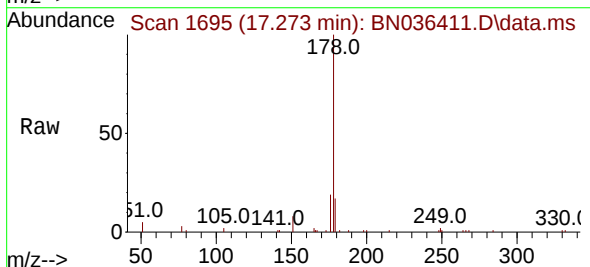


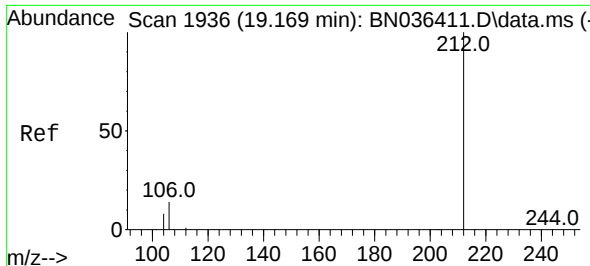

#27
Fluoranthene-d10
Concen: 0.413 ng
RT: 19.169 min Scan# 1936
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:212 Resp: 8851
Ion Ratio Lower Upper
212 100
106 14.4 11.5 17.3
104 8.9 7.1 10.7

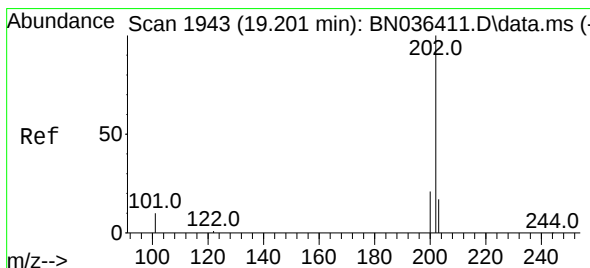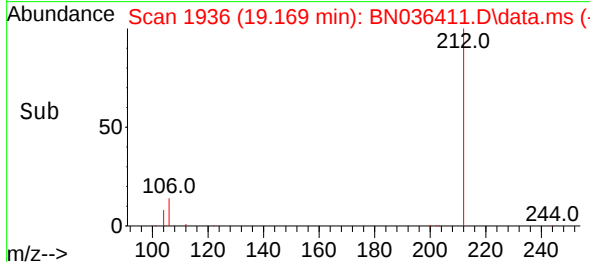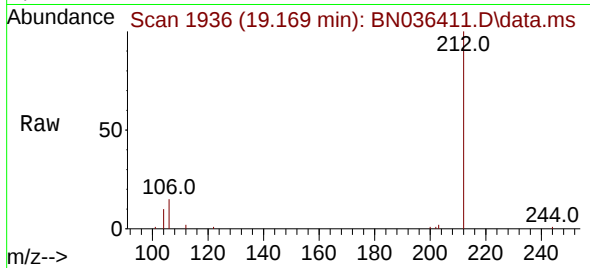

#28
Fluoranthene
Concen: 0.389 ng
RT: 19.201 min Scan# 1943
Delta R.T. 0.000 min
Lab File: BN036411.D
Acq: 10 Feb 2025 13:36

Tgt Ion:202 Resp: 11264
Ion Ratio Lower Upper
202 100
101 11.5 9.2 13.8
203 16.7 13.4 20.0

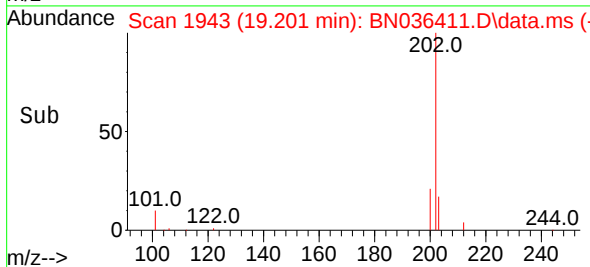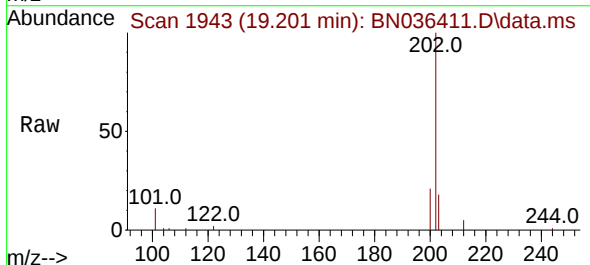

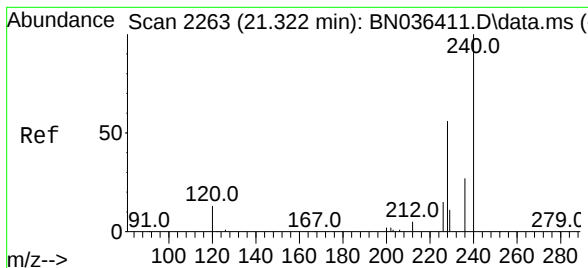

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.322 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:240 Resp: 7484

Ion Ratio Lower Upper

240 100

120 16.6 13.3 19.9

236 28.8 23.0 34.6

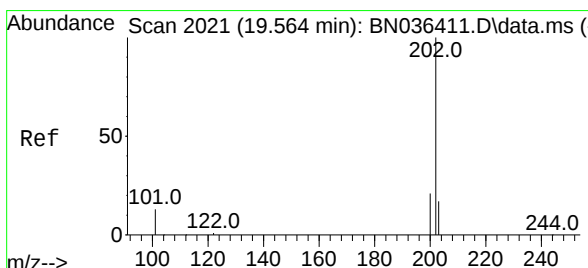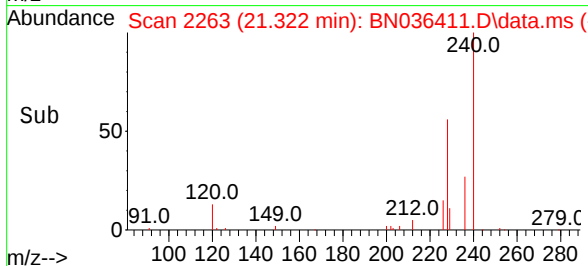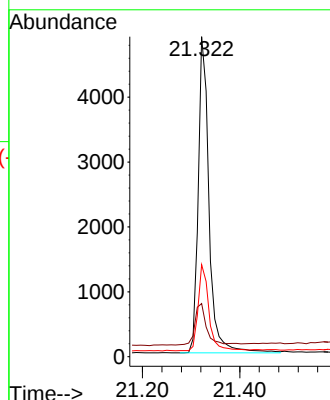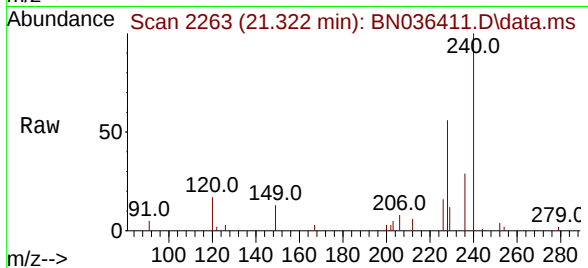

#30

Pyrene

Concen: 0.384 ng

RT: 19.564 min Scan# 2021

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36




Tgt Ion:202 Resp: 11479


Ion Ratio Lower Upper

202 100

200 21.1 16.9 25.3

203 17.4 13.9 20.9

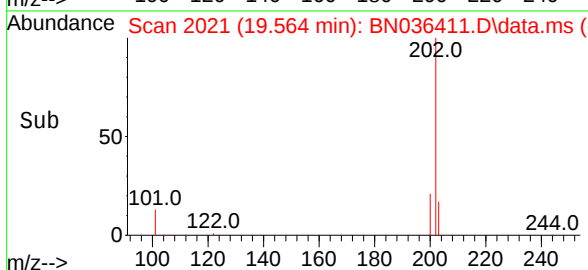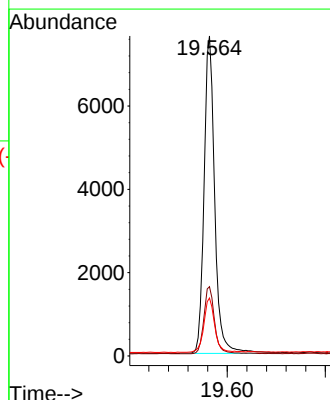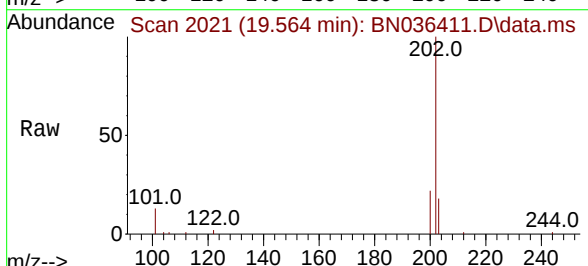



#31

Terphenyl-d14

Concen: 0.412 ng

RT: 19.768 min Scan# 2065

Delta R.T. 0.000 min

Lab File: BN036411.D


Acq: 10 Feb 2025 13:36

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4






Tgt Ion:244 Resp: 6378

Ion Ratio Lower Upper

244 100

212 10.1 8.1 12.1

122 16.0 12.8 19.2

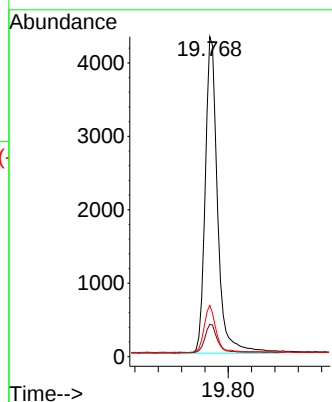

#32

Benzo(a)anthracene

Concen: 0.364 ng

RT: 21.313 min Scan# 2262

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36




Tgt Ion:228 Resp: 9677


Ion Ratio Lower Upper

228 100

226 27.7 22.2 33.2

229 20.6 16.5 24.7

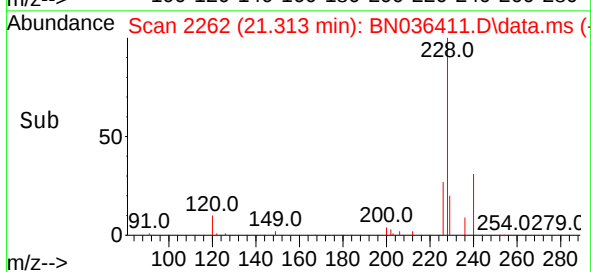




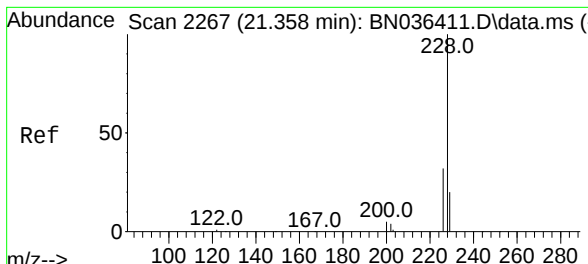


#33
 Chrysene
 Concen: 0.373 ng
 RT: 21.358 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN036411.D
 Acq: 10 Feb 2025 13:36

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion: 228 Resp: 10178




Ion	Ratio	Lower	Upper
228	100		
226	31.9	25.5	38.3
229	20.5	16.4	24.6

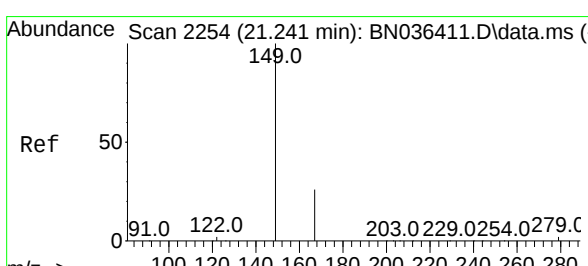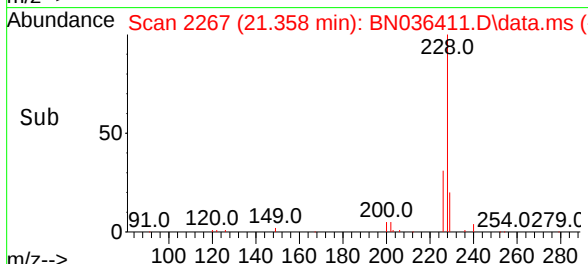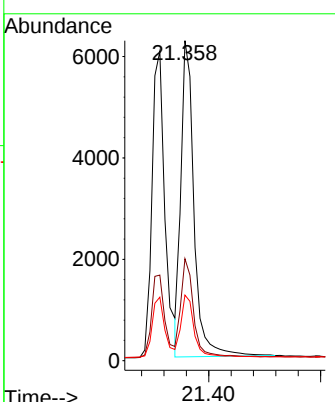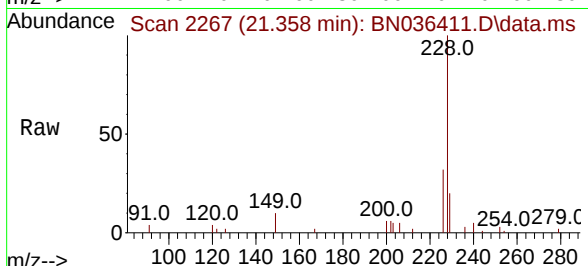


#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.392 ng
 RT: 21.241 min Scan# 2254
 Delta R.T. 0.000 min
 Lab File: BN036411.D
 Acq: 10 Feb 2025 13:36

Tgt Ion: 149 Resp: 5815

Ion	Ratio	Lower	Upper
149	100		
167	26.5	21.2	31.8
279	3.4	2.7	4.1

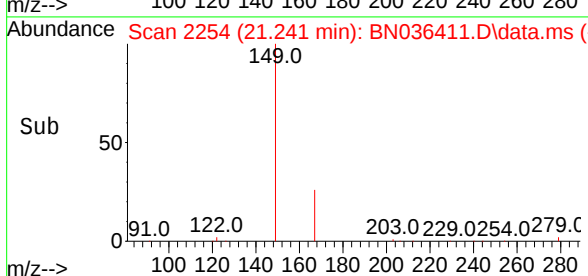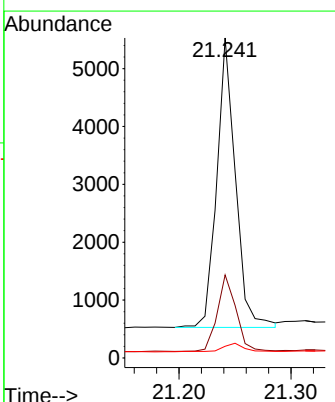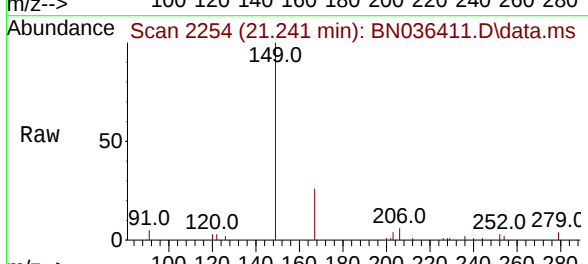



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.595 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:264 Resp: 7735

Ion Ratio Lower Upper

264 100

260 26.1 20.9 31.3

265 75.9 60.7 91.1

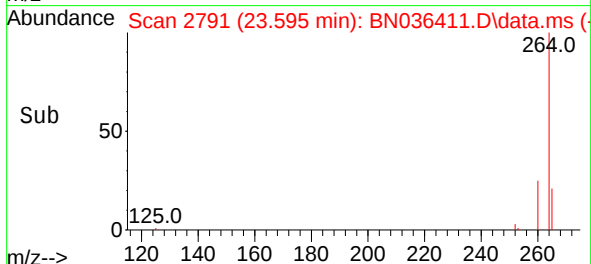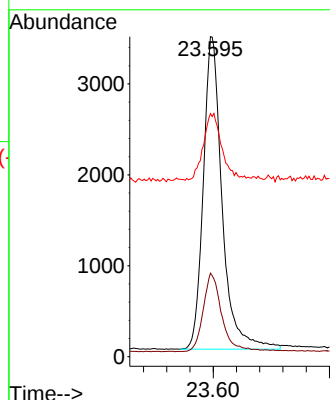

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.351 ng

RT: 25.899 min Scan# 3579

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36




Tgt Ion:276 Resp: 10661


Ion Ratio Lower Upper

276 100

138 27.8 22.2 33.2

277 24.8 19.8 29.6

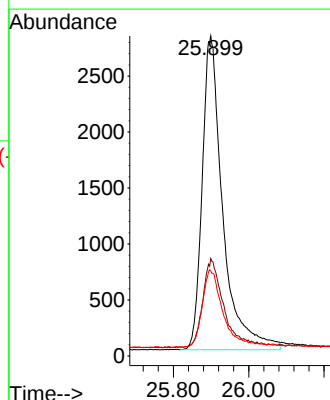



#37

Benzo(b)fluoranthene

Concen: 0.355 ng

RT: 22.911 min Scan# 2557

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:252 Resp: 9743

Ion Ratio Lower Upper

252 100

253 27.4 21.9 32.9

125 18.8 15.0 22.6

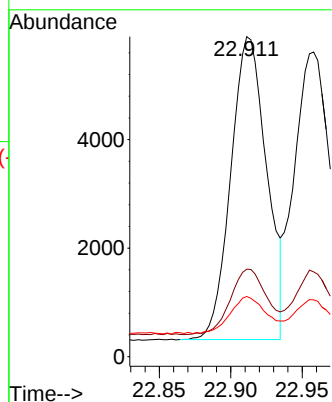

#38

Benzo(k)fluoranthene

Concen: 0.377 ng

RT: 22.958 min Scan# 2573

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36




Tgt Ion:252 Resp: 10543


Ion Ratio Lower Upper

252 100

253 27.8 22.2 33.4

125 18.7 15.0 22.4





#39

Benzo(a)pyrene

Concen: 0.362 ng

RT: 23.499 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN036411.D


Acq: 10 Feb 2025 13:36

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4






Tgt Ion:252 Resp: 8521

Ion Ratio Lower Upper

252 100

253 30.5 24.4 36.6

125 22.7 18.2 27.2

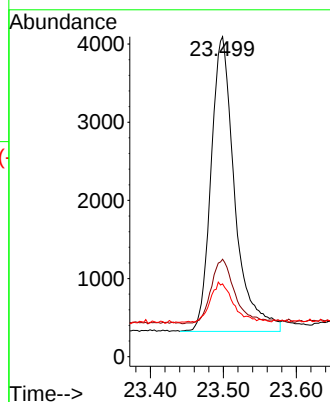

#40

Dibenzo(a,h)anthracene

Concen: 0.344 ng

RT: 25.917 min Scan# 3585

Delta R.T. 0.000 min

Lab File: BN036411.D

Acq: 10 Feb 2025 13:36




Tgt Ion:278 Resp: 8314


Ion Ratio Lower Upper

278 100

139 23.1 18.5 27.7

279 31.0 24.8 37.2

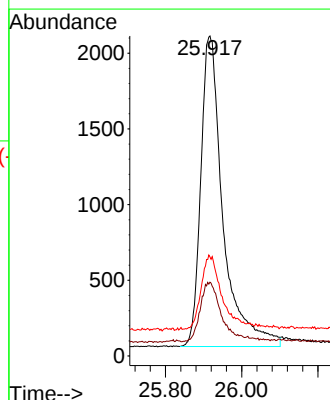

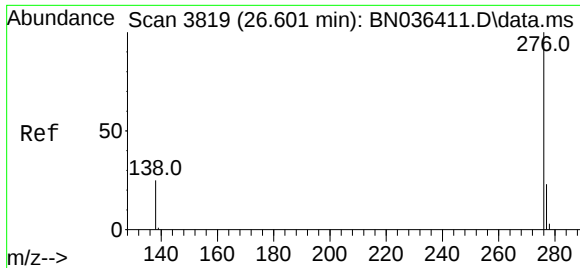

#41

Benzo(g,h,i)perylene

Concen: 0.366 ng

RT: 26.601 min Scan# 3819

Delta R.T. 0.000 min

Lab File: BN036411.D


Acq: 10 Feb 2025 13:36

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4

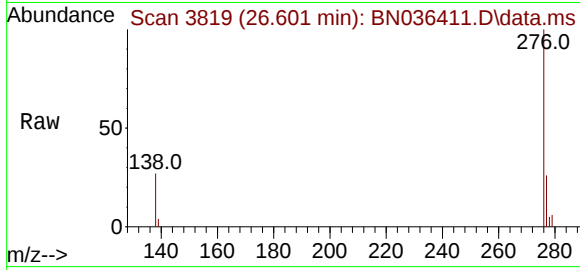

Tgt Ion:276 Resp: 9701

Ion Ratio Lower Upper

276 100

277 25.9 20.7 31.1

138 27.2 21.8 32.6

