
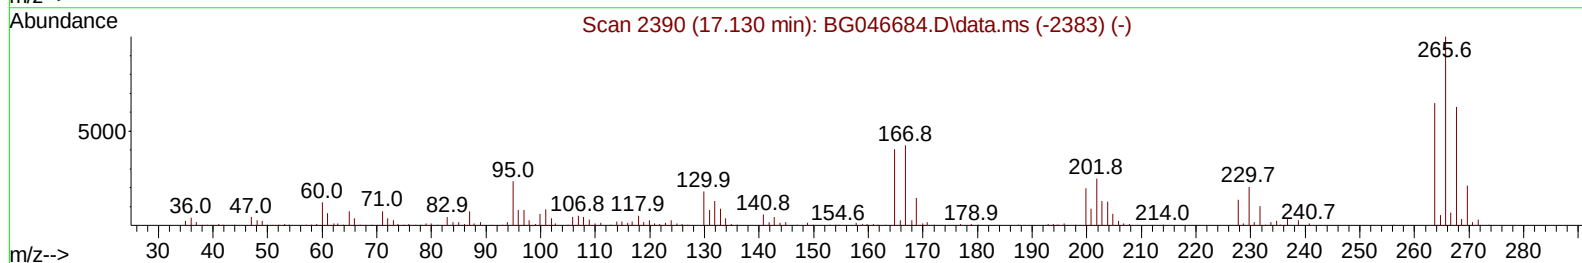
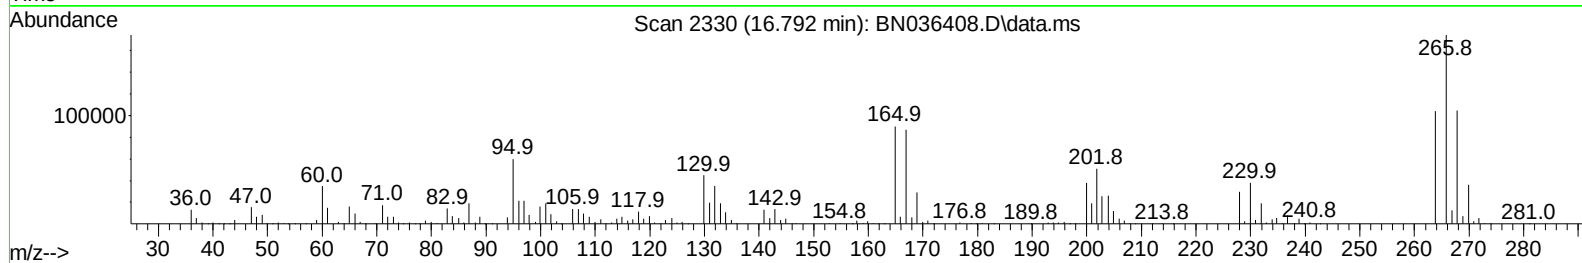


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021025\
Data File : BN036408.D
Acq On : 10 Feb 2025 11:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 01:55:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

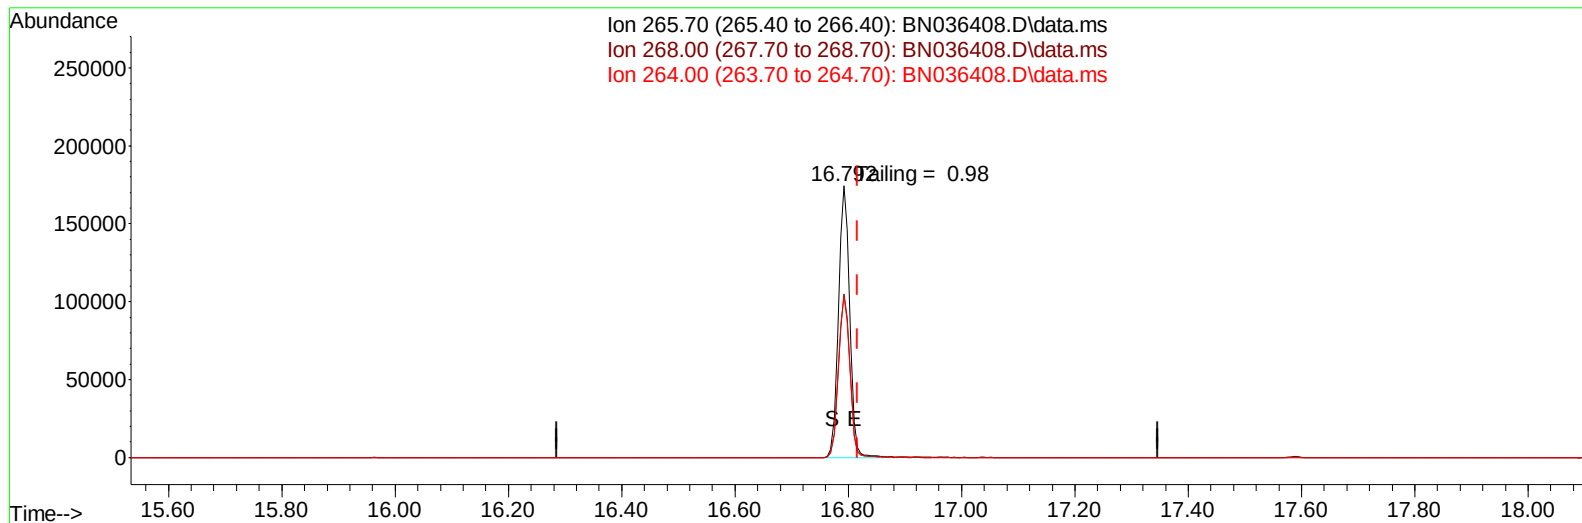




TIC: BN036408.D\data.ms

(70) Pentachlorophenol (C)**16.792min (-0.024) 22697.76 ng****response 239758**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.20
264.00	61.60	59.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021025\
Data File : BN036408.D
Acq On : 10 Feb 2025 11:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 01:55:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

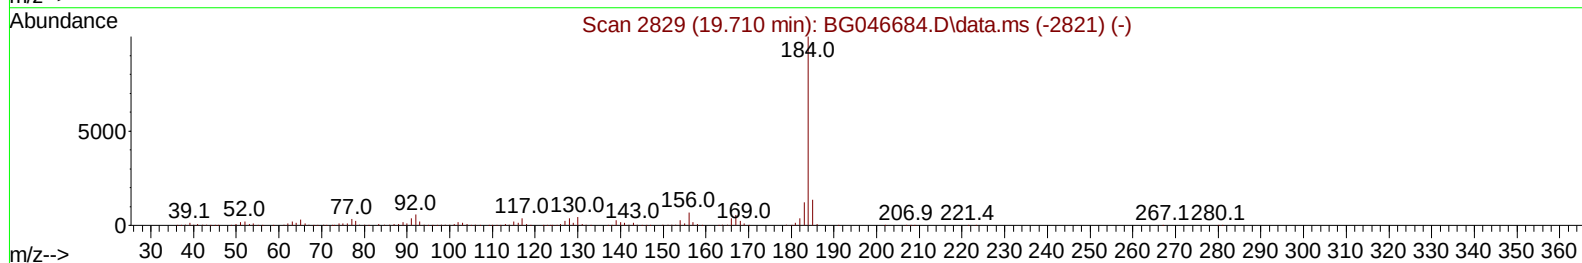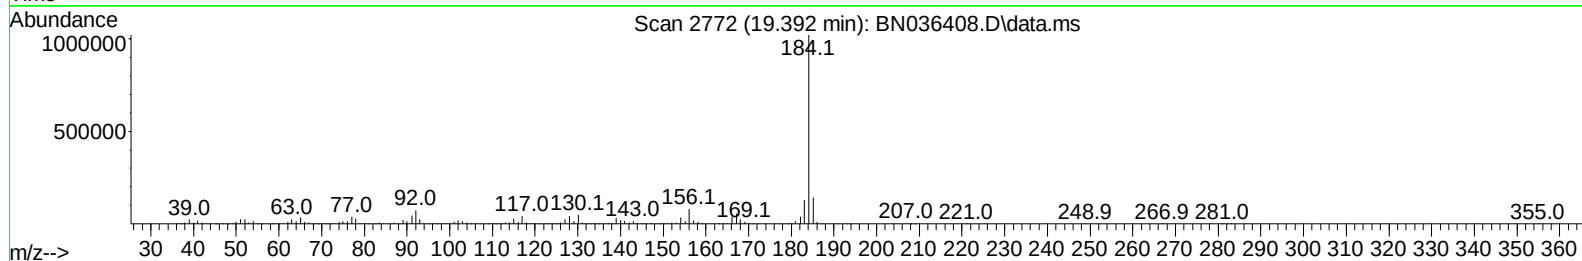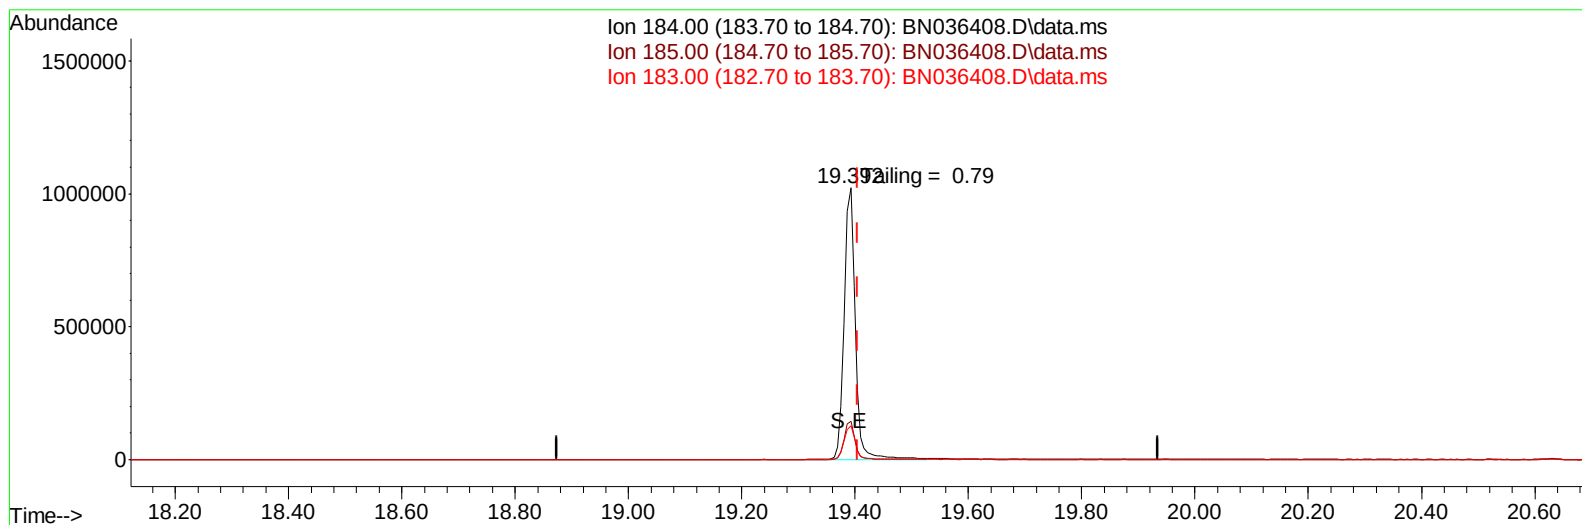

TIC: BN036408.D\data.ms

(77) Benzidine

19.392min (-0.012) 0.00 ng

response 1390167

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.06
183.00	13.20	12.43
0.00	0.00	0.00