
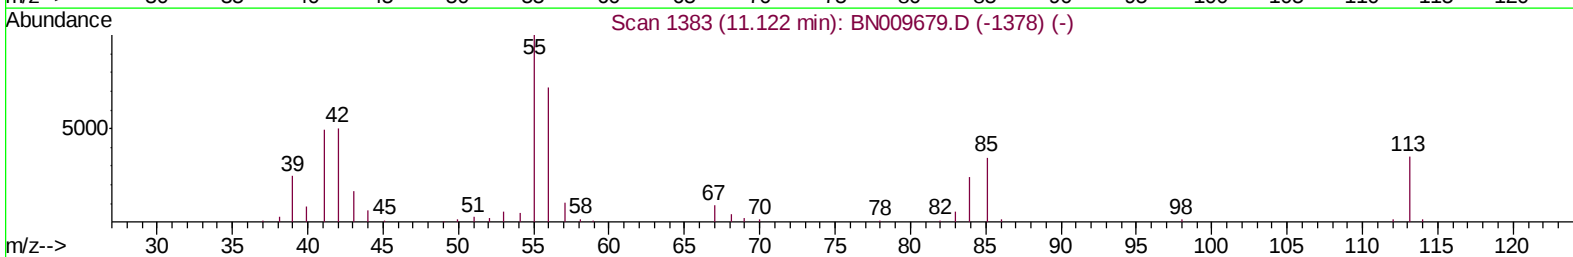
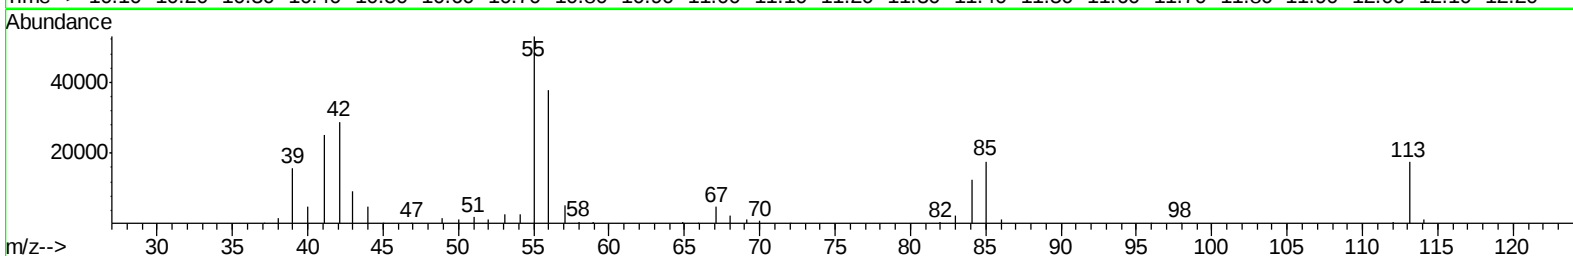


Data File : BN009701.D
Acq On : 11 Feb 2020 10:48
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 12 00:43:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 15:21:46 2020
Response via : Initial Calibration

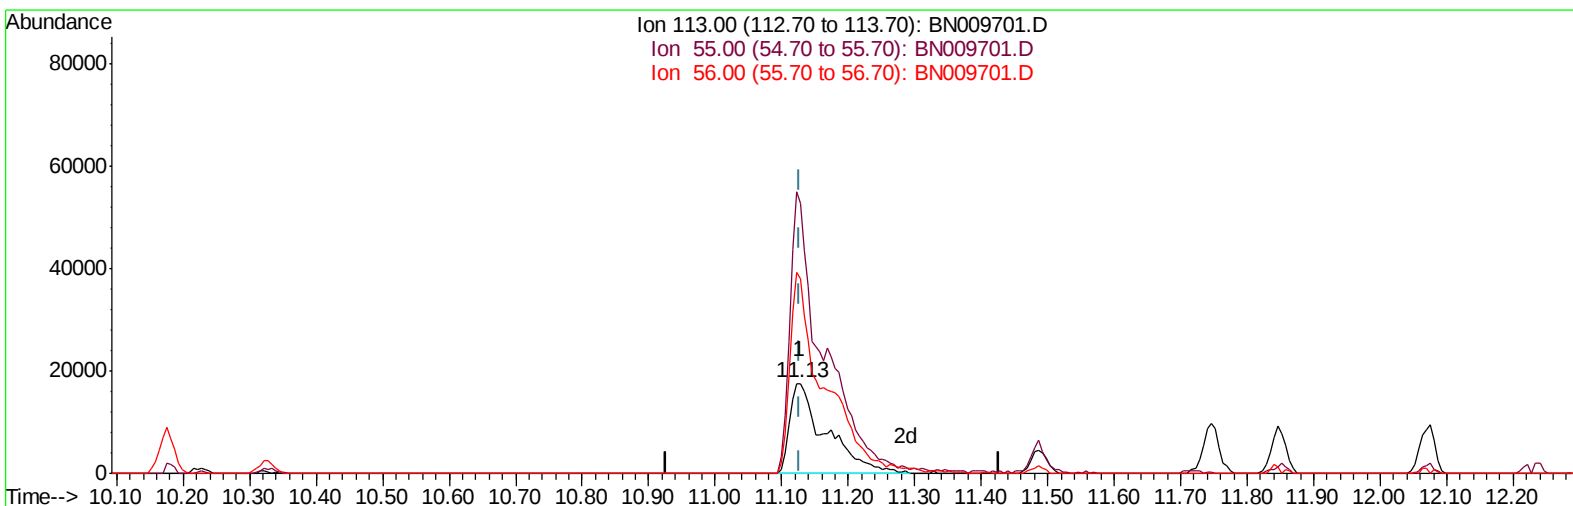

TIC: BN009701.D

(32) Caprolactam

11.128min (+0.000) 17.97ng/ul m

response 66919

Ion	Exp%	Act%
113.00	100	100
55.00	258.80	300.41
56.00	199.10	215.50
0.00	0.00	0.00