
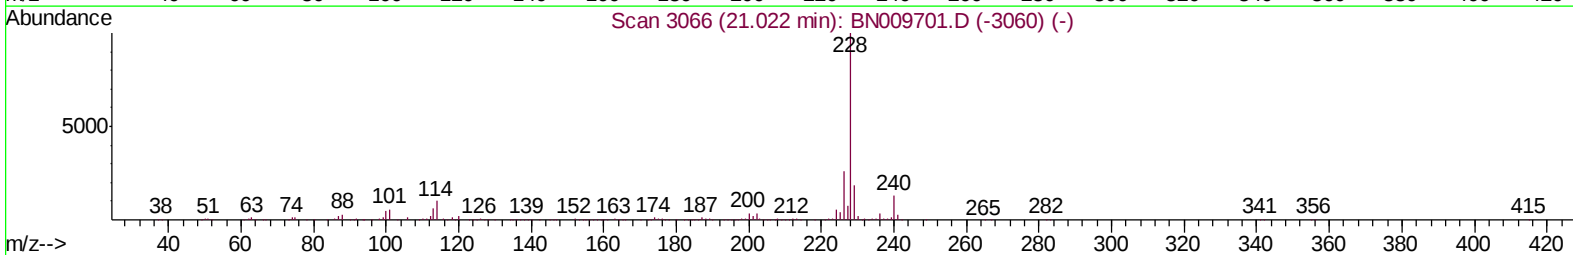
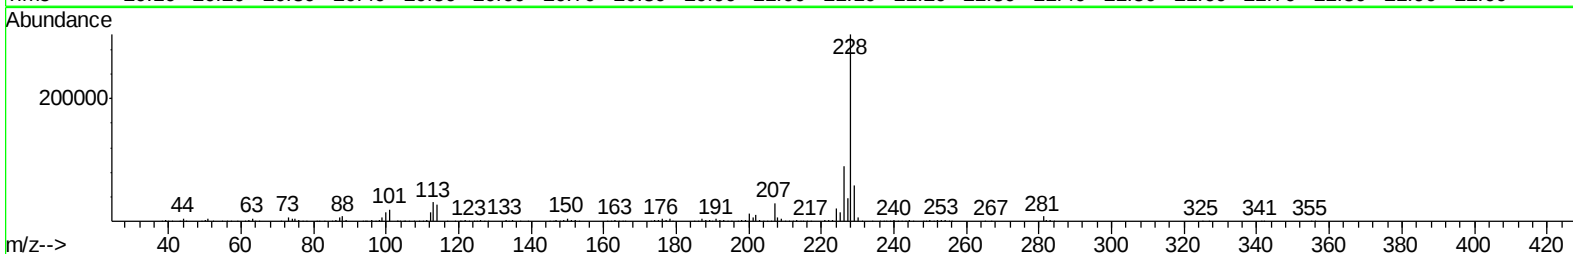


Data File : BN009702.D
Acq On : 11 Feb 2020 11:51
Operator : CG/JU
Sample : L1324-04MEDL 10X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Feb 12 00:54:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 00:52:44 2020
Response via : Initial Calibration

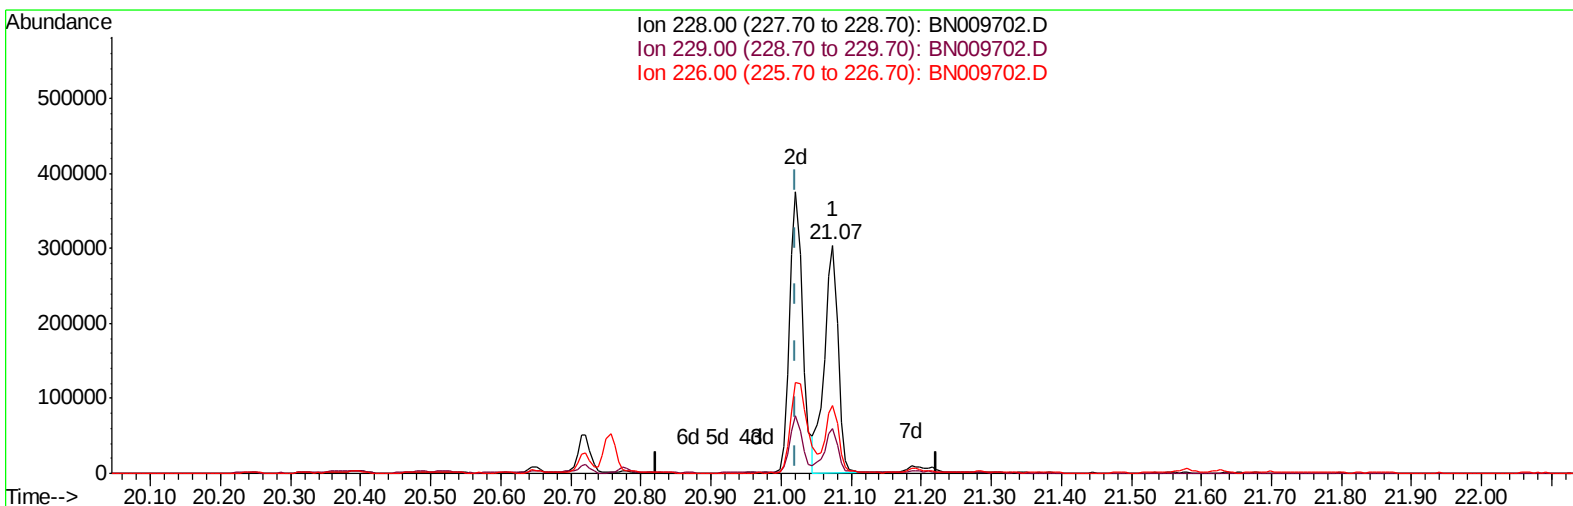

TIC: BN009702.D

(82) Benzo(a)anthracene
21.074min (+0.053) 8.42ng/ul
response 408161

Ion	Exp%	Act%
228.00	100	100
229.00	18.70	19.57
226.00	26.10	29.49
0.00	0.00	0.00