

Data File : BN009702.D

Acq On : 11 Feb 2020 11:51

Operator : CG/JU

Sample : L1324-04MEDL 10X

Misc :

ALS Vial : 3 Sample Multiplier: 1




Quant Time: Feb 12 00:54:49 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Feb 12 00:52:44 2020

Response via : Initial Calibration

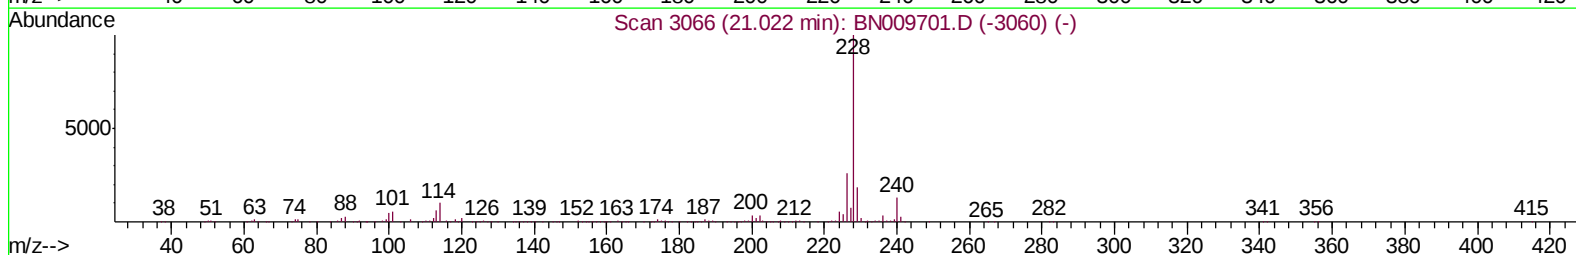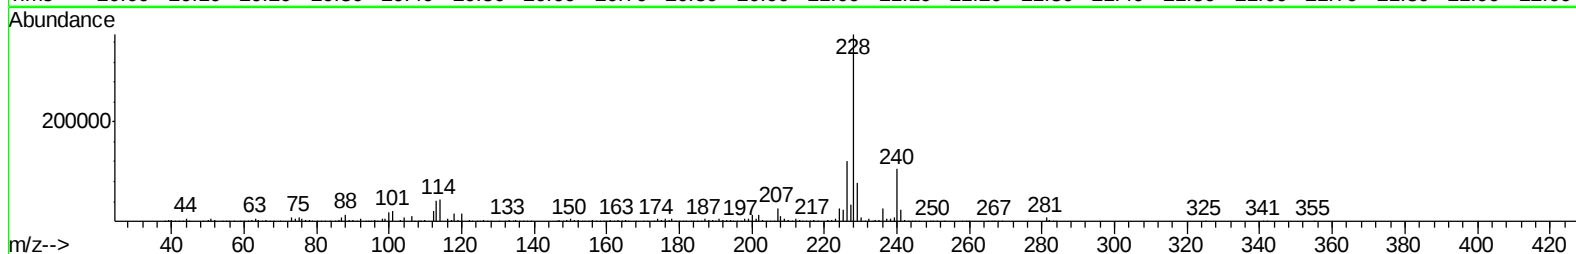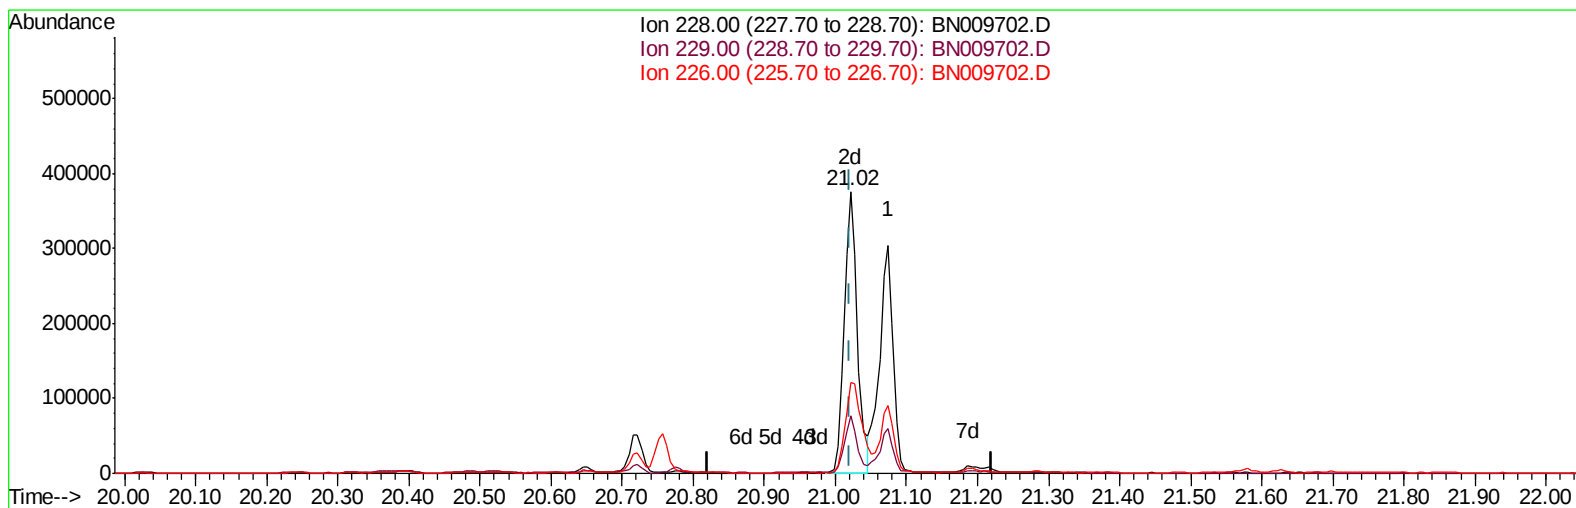

TIC: BN009702.D

(82) Benzo(a)anthracene

21.021min (-0.000) 10.01ng/ul m

response 485050

Ion	Exp%	Act%
228.00	100	100
229.00	18.70	20.44
226.00	26.10	32.11#
0.00	0.00	0.00