
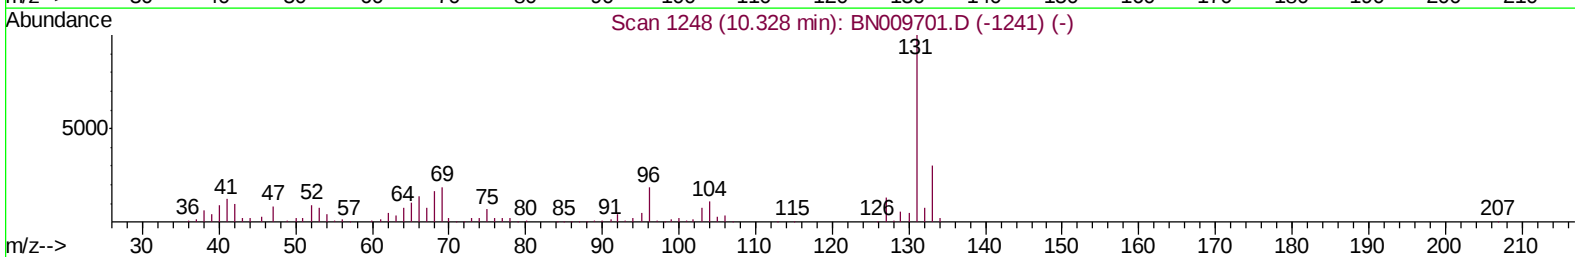
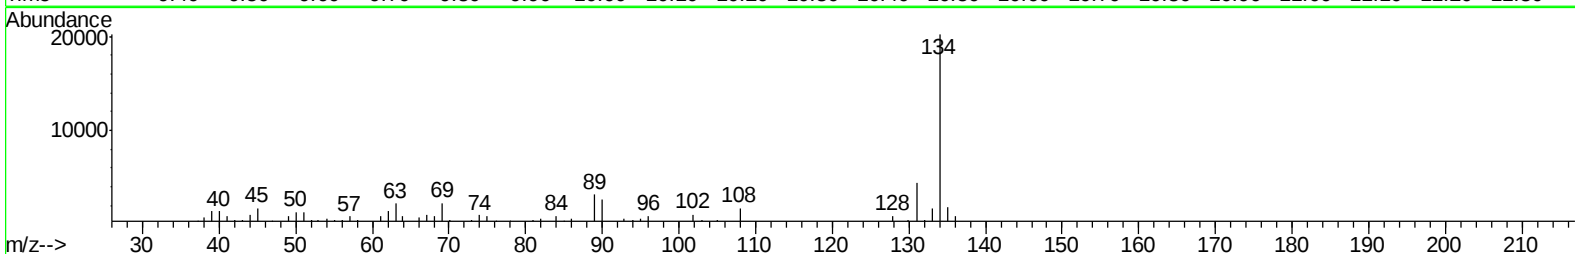


Data File : BN009702.D
Acq On : 11 Feb 2020 11:51
Operator : CG/JU
Sample : L1324-04MEDL 10X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Feb 12 01:11:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 00:52:44 2020
Response via : Initial Calibration

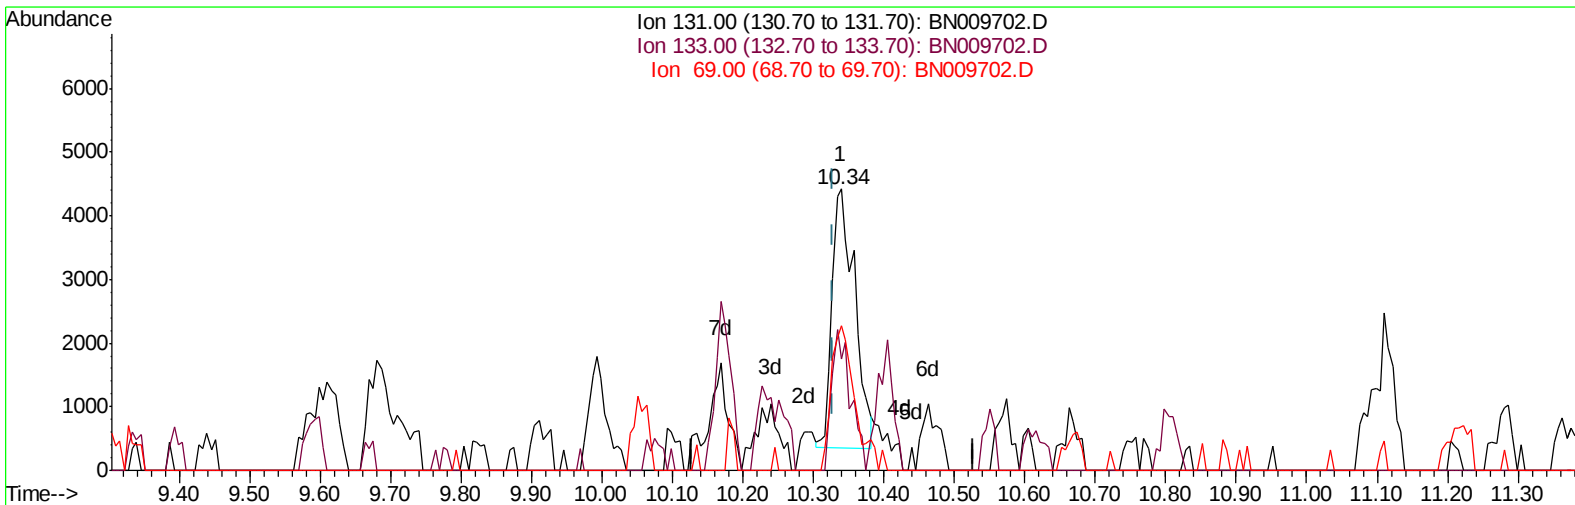

TIC: BN009702.D

(29) 4-Chloroaniline-d4 (S)

10.340min (+0.011) 1.01ng/ul m

response 8974

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	39.37#
69.00	21.00	51.34#
0.00	0.00	0.00