
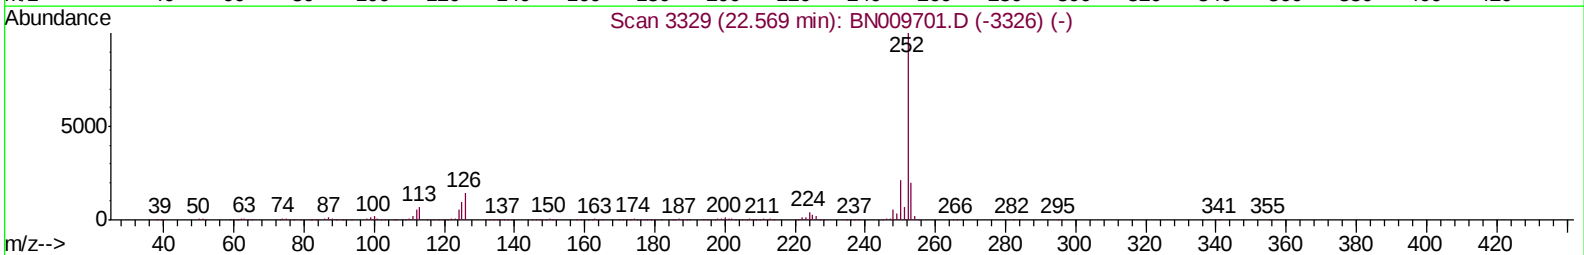
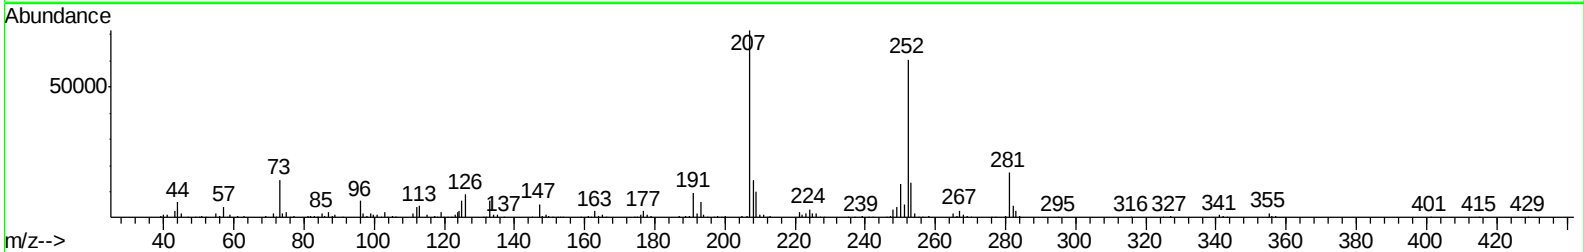


Data File : BN009703.D
Acq On : 11 Feb 2020 12:51
Operator : CG/JU
Sample : L1324-15MEDL 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Feb 12 00:54:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 00:52:44 2020
Response via : Initial Calibration

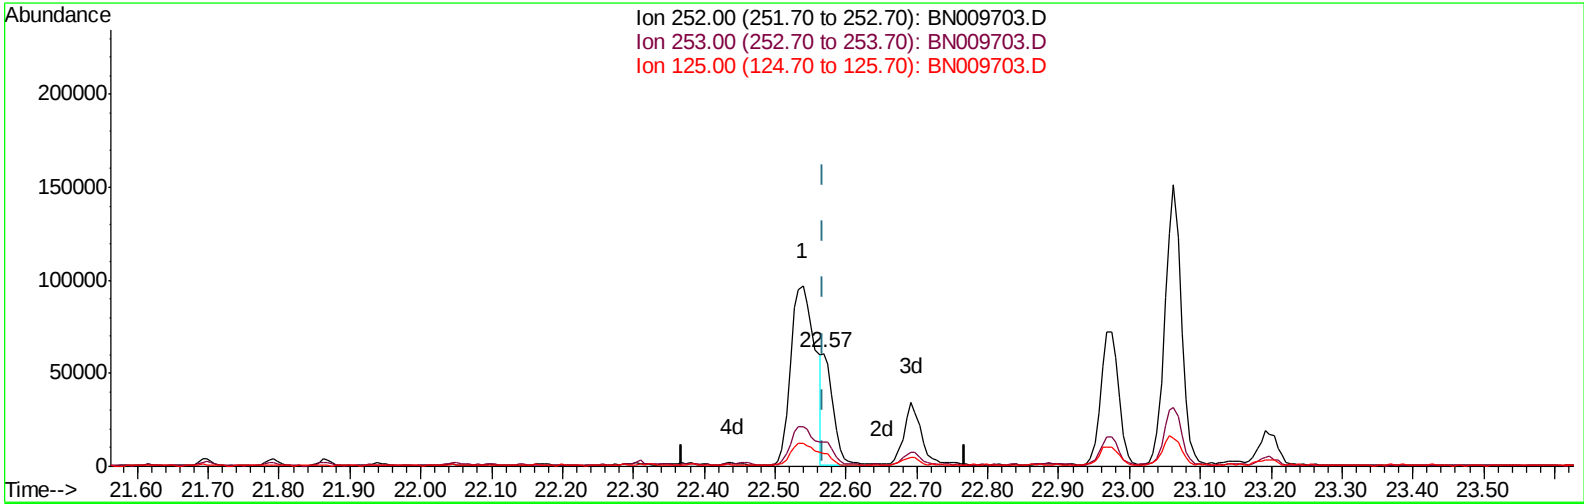

TIC: BN009703.D

(88) Benzo(k)fluoranthene

22.568min (-0.000) 1.31ng/ul m

response 66672

Ion	Exp%	Act%
252.00	100	100
253.00	21.20	22.08
125.00	10.00	11.28
0.00	0.00	0.00