
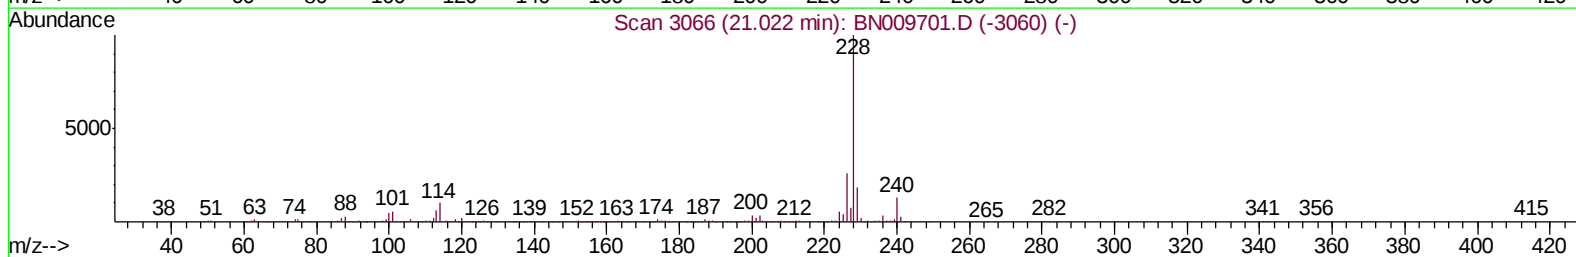
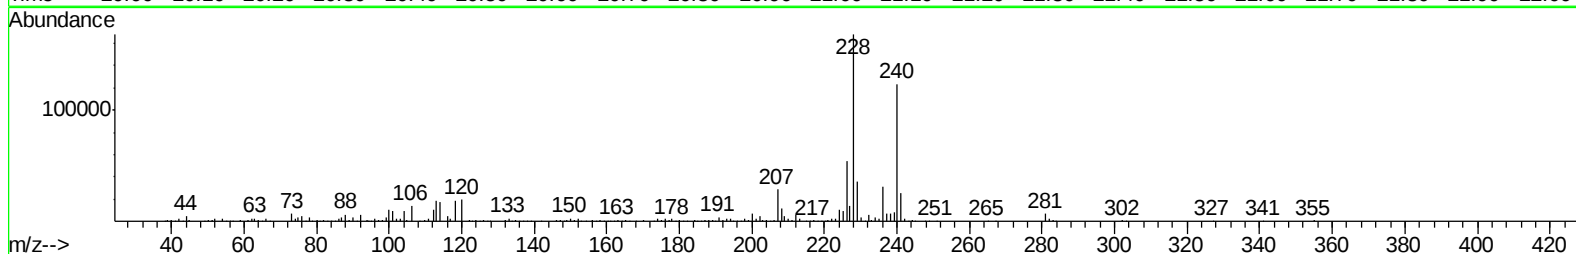


Data File : BN009704.D
Acq On : 11 Feb 2020 13:34
Operator : CG/JU
Sample : L1324-16MEDL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Feb 12 00:55:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 00:52:44 2020
Response via : Initial Calibration

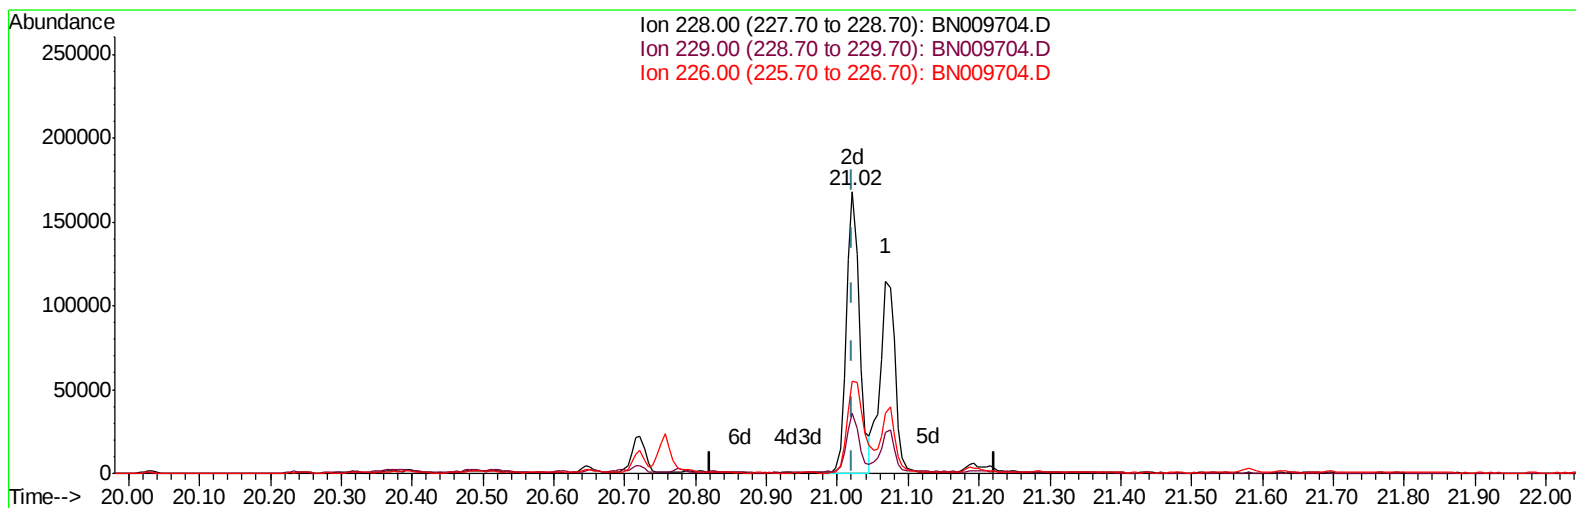

TIC: BN009704.D

(82) Benzo(a)anthracene

21.022min (+0.000) 3.78ng/ul m

response 215577

Ion	Exp%	Act%
228.00	100	100
229.00	18.70	21.20
226.00	26.10	32.60#
0.00	0.00	0.00