
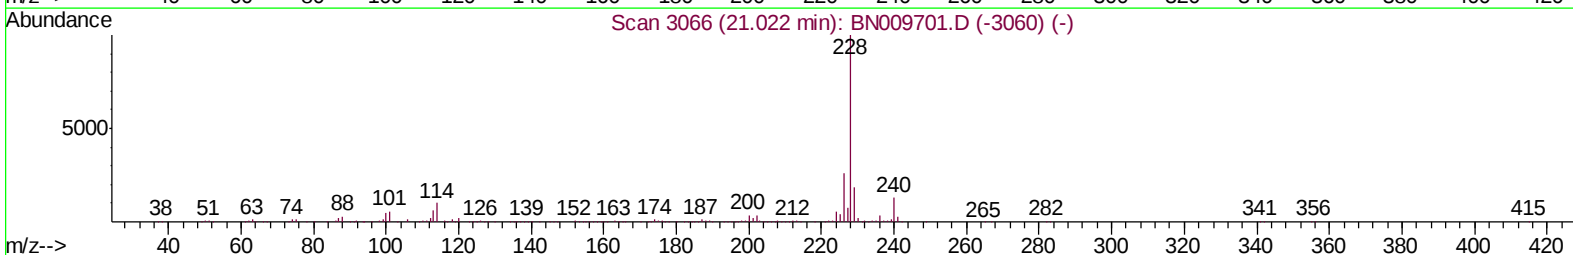
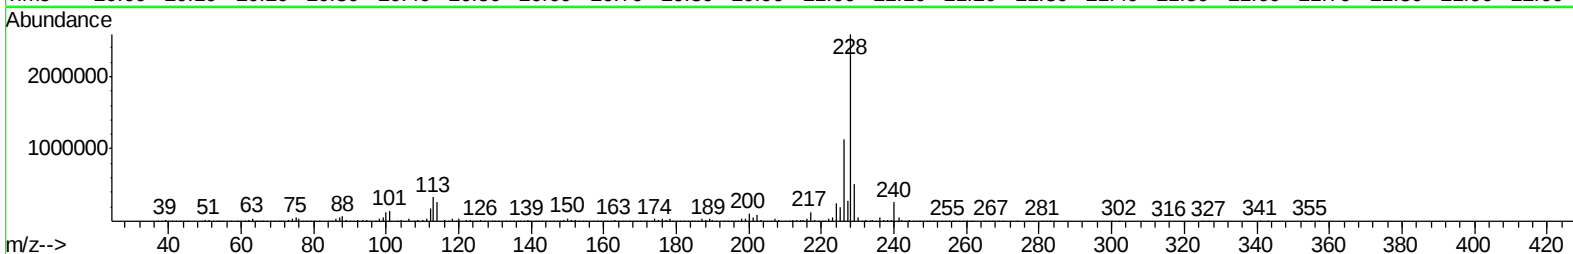


Data File : BN009705.D
Acq On : 11 Feb 2020 14:24
Operator : CG/JU
Sample : L1324-05ME
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Feb 12 00:55:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 00:52:44 2020
Response via : Initial Calibration

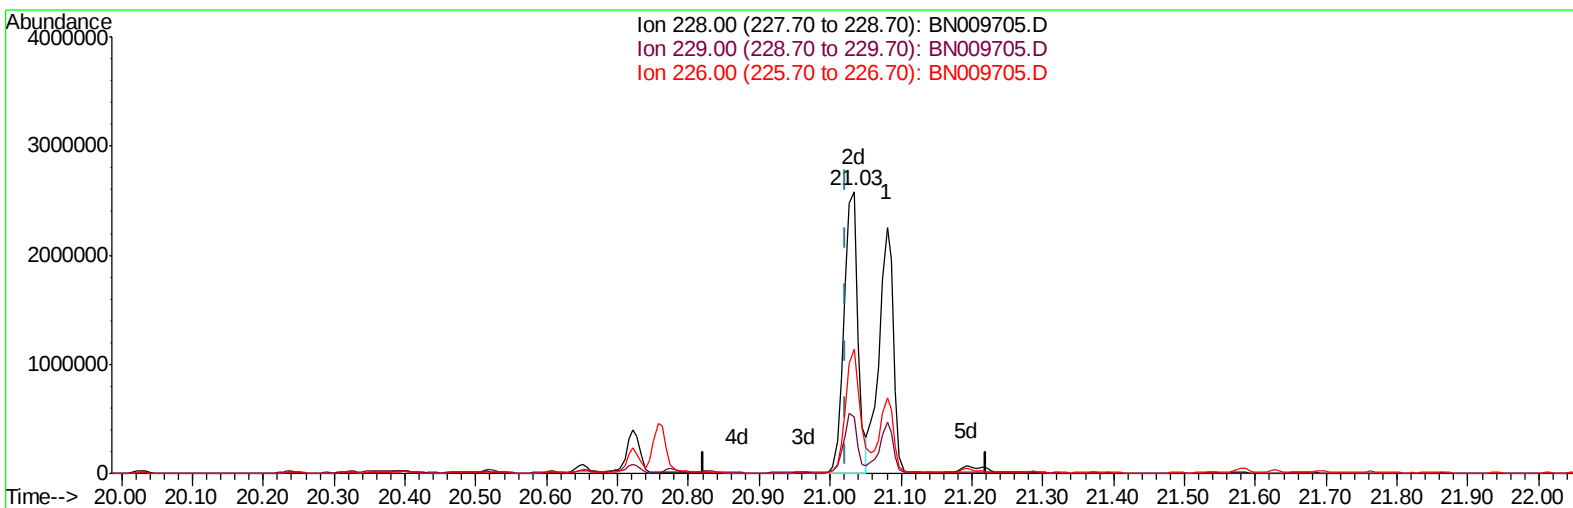

TIC: BN009705.D

(82) Benzo(a)anthracene

21.033min (+0.012) 72.34ng/ul m

response 3525203

Ion	Exp%	Act%
228.00	100	100
229.00	18.70	19.86
226.00	26.10	43.96#
0.00	0.00	0.00