
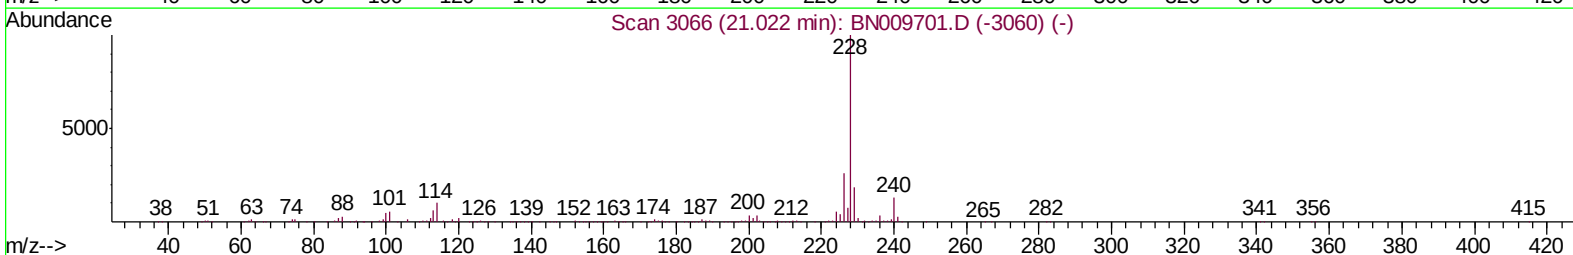
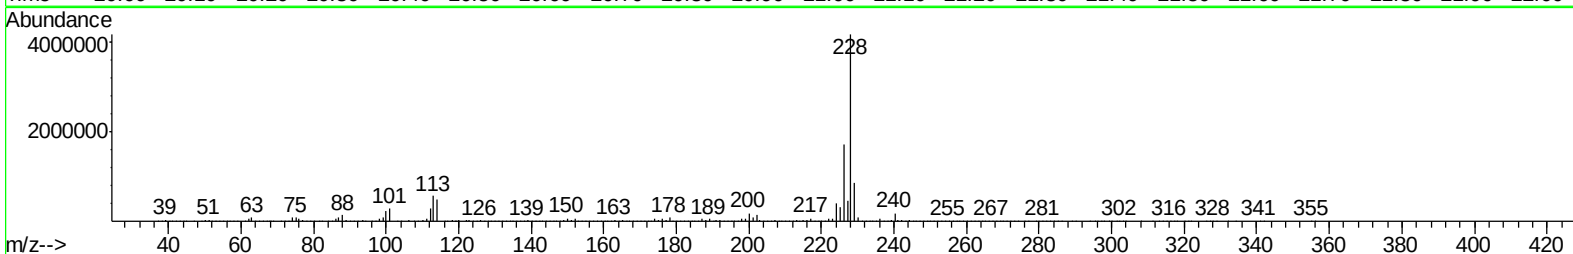


Data File : BN009706.D
Acq On : 11 Feb 2020 15:50
Operator : CG/JU
Sample : L1324-14 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 12 02:33:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 00:52:44 2020
Response via : Initial Calibration

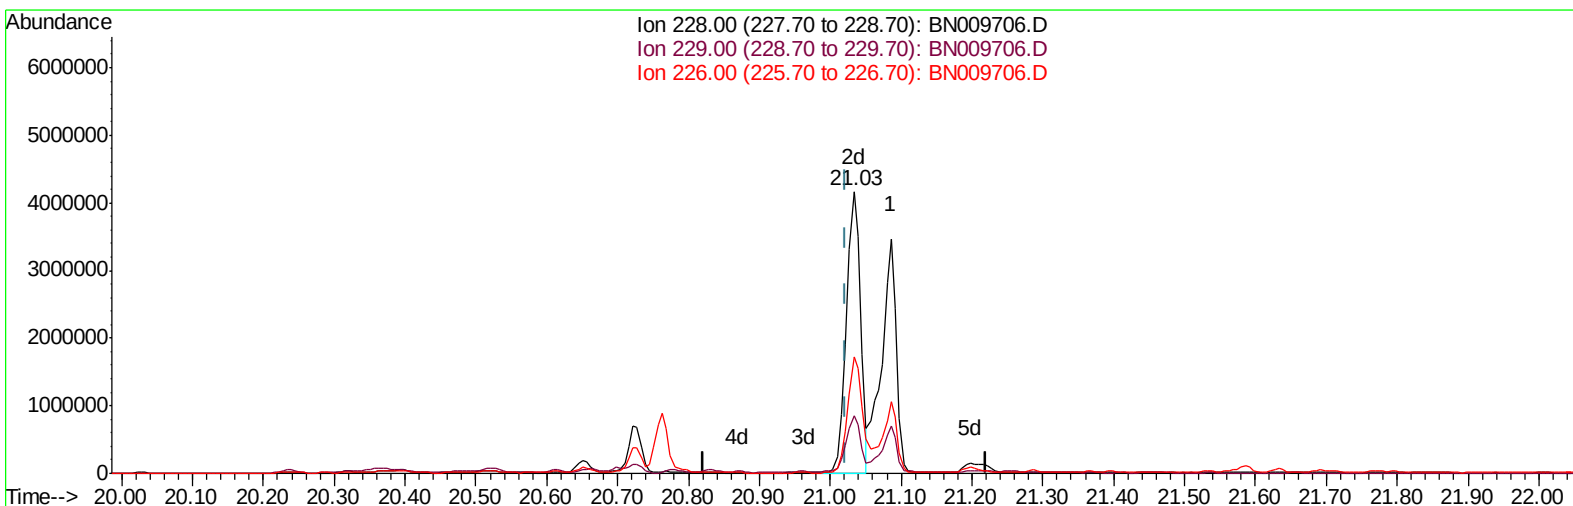

TIC: BN009706.D

(82) Benzo(a)anthracene

21.033min (+0.012) 70.59ng/ul m

response 5830370

Ion	Exp%	Act%
228.00	100	100
229.00	18.70	20.54
226.00	26.10	41.20#
0.00	0.00	0.00