

Data File : BN009706.D

Acq On : 11 Feb 2020 15:50

Operator : CG/JU

Sample : L1324-14 10X

Misc :

ALS Vial : 7 Sample Multiplier: 1




Quant Time: Feb 12 02:33:32 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Feb 12 00:52:44 2020

Response via : Initial Calibration

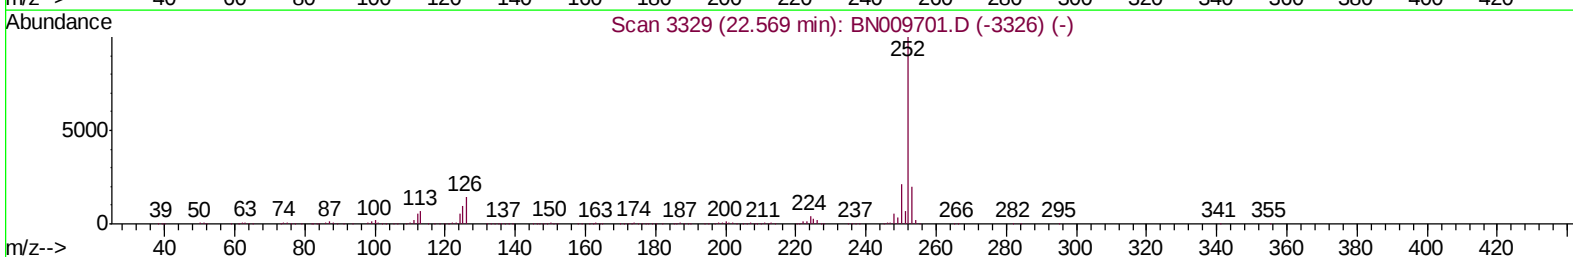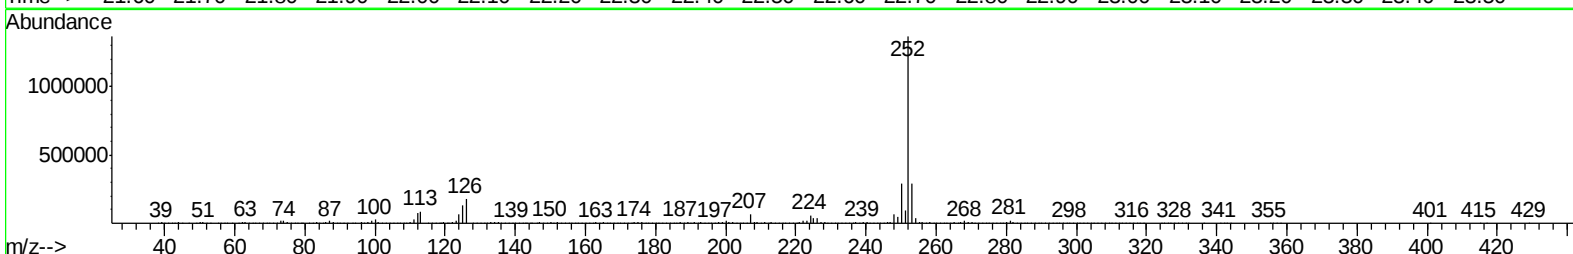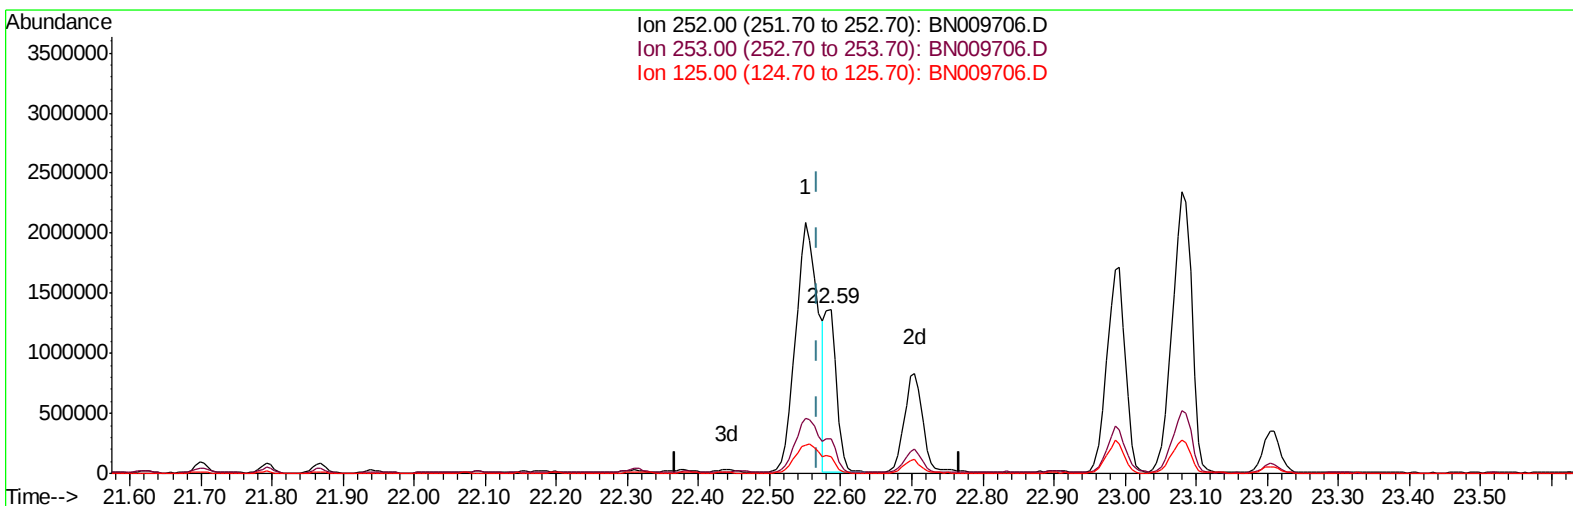

TIC: BN009706.D

(88) Benzo(k)fluoranthene

22.586min (+0.018) 19.49ng/ul m

response 1519995

Ion	Exp%	Act%
252.00	100	100
253.00	21.20	20.98
125.00	10.00	9.78
0.00	0.00	0.00