
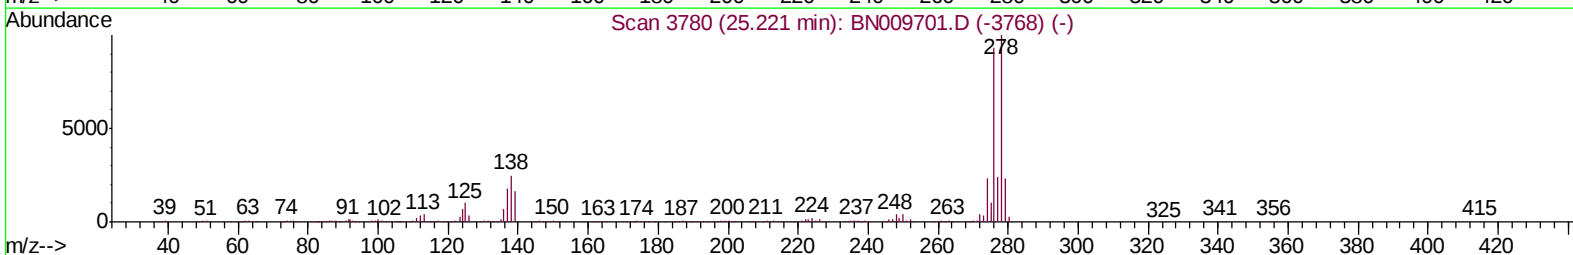
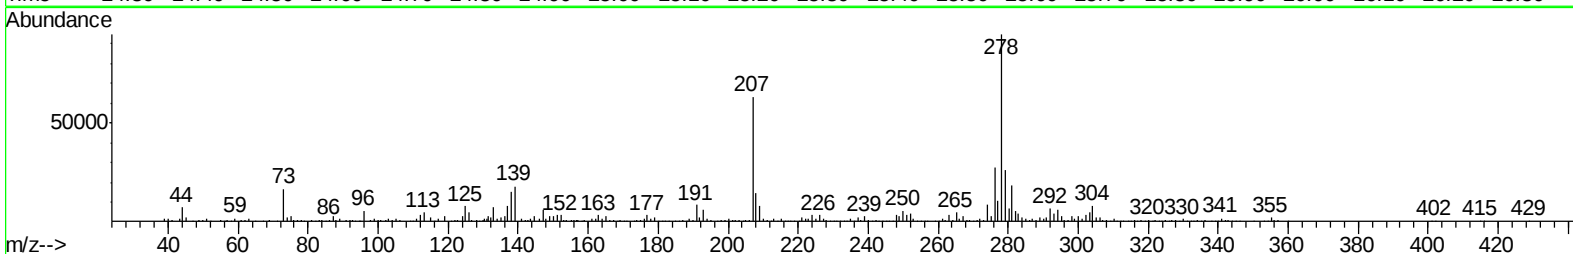


Data File : BN009706.D
Acq On : 11 Feb 2020 15:50
Operator : CG/JU
Sample : L1324-14 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Feb 12 02:33:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 00:52:44 2020
Response via : Initial Calibration

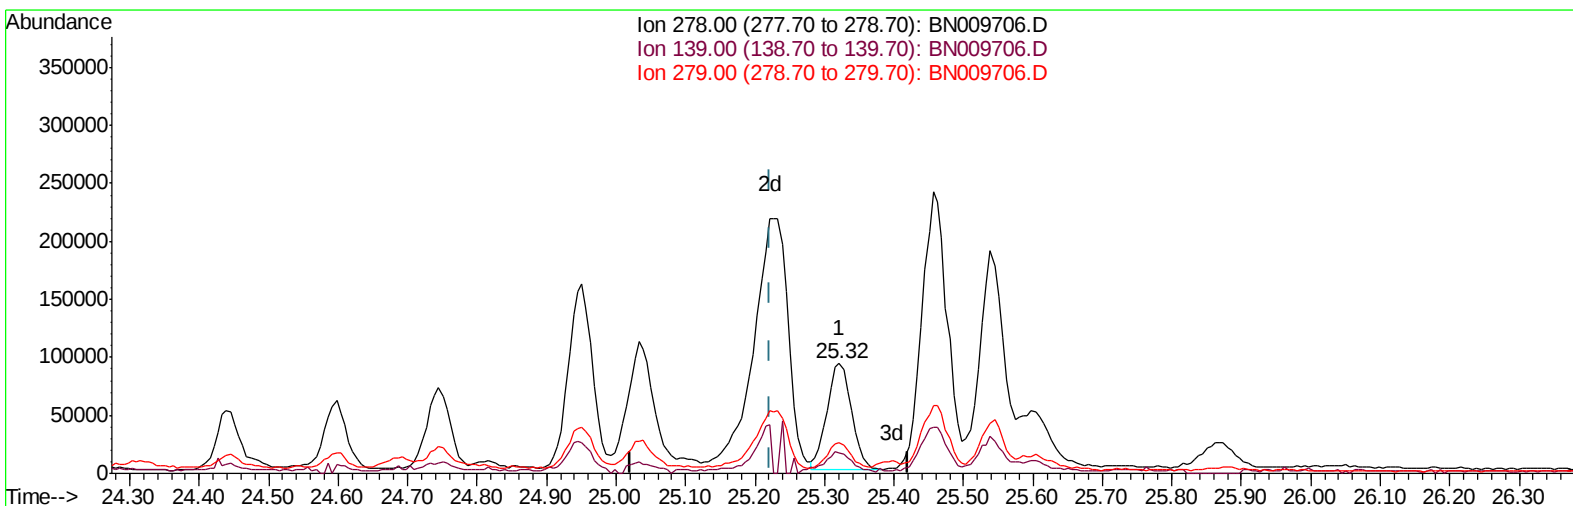

TIC: BN009706.D

(92) Dibenzo(a,h)anthracene

25.321min (+0.100) 3.06ng/ul

response 225011

Ion	Exp%	Act%
278.00	100	100
139.00	15.90	19.05
279.00	24.80	27.87
0.00	0.00	0.00