
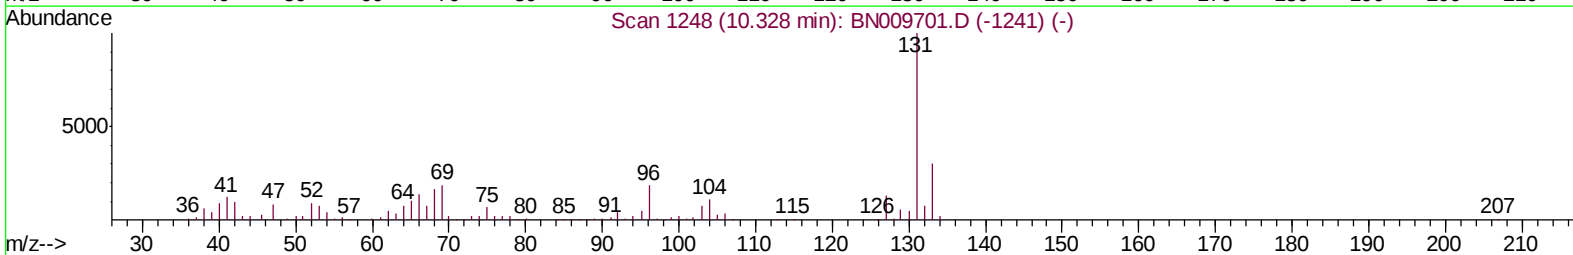
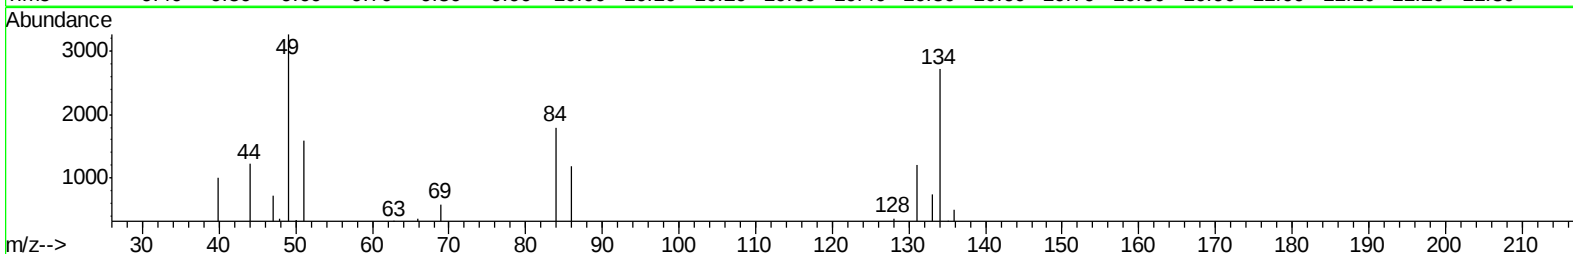


Data File : BN009708.D
Acq On : 11 Feb 2020 17:31
Operator : CG/JU
Sample : L1324-05MEDL2 40X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 12 00:56:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 00:52:44 2020
Response via : Initial Calibration

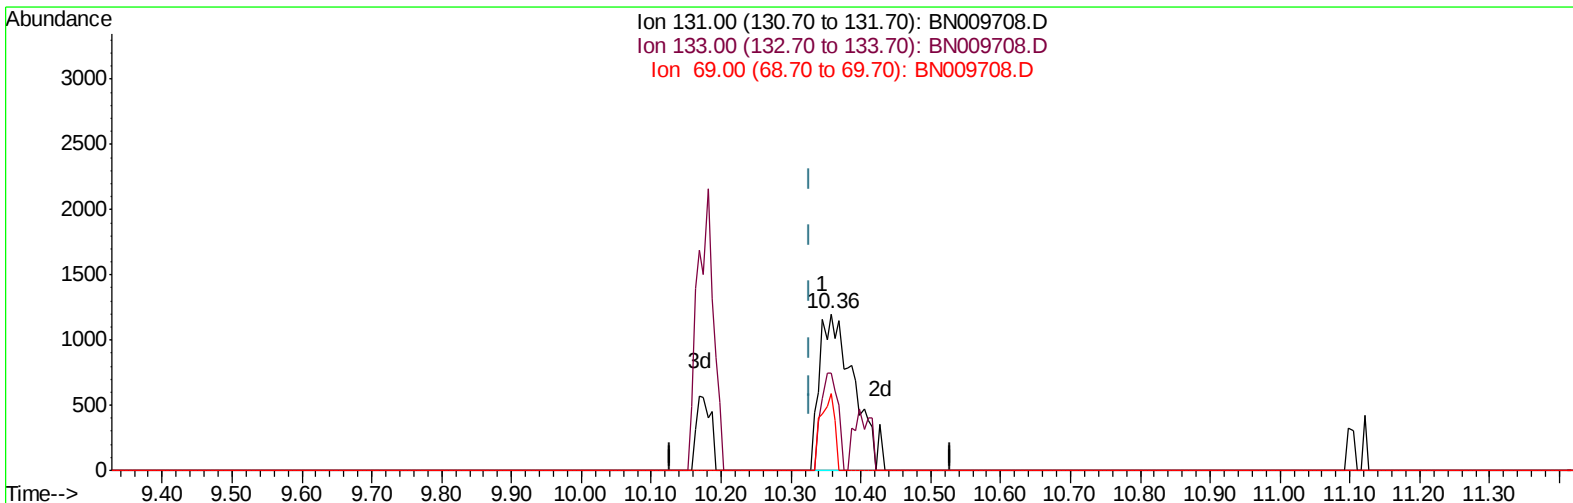

TIC: BN009708.D

(29) 4-Chloroaniline-d4 (S)

10.357min (+0.029) 0.47ng/ul m

response 3963

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	61.76#
69.00	21.00	48.79#
0.00	0.00	0.00