
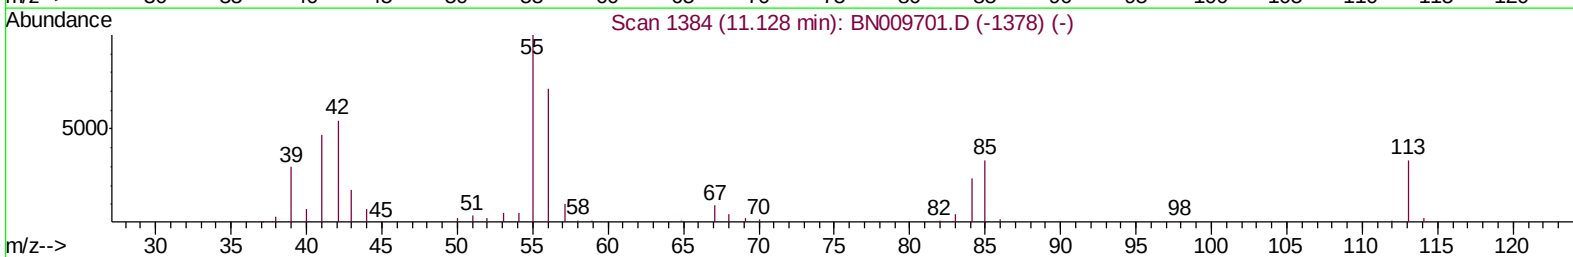
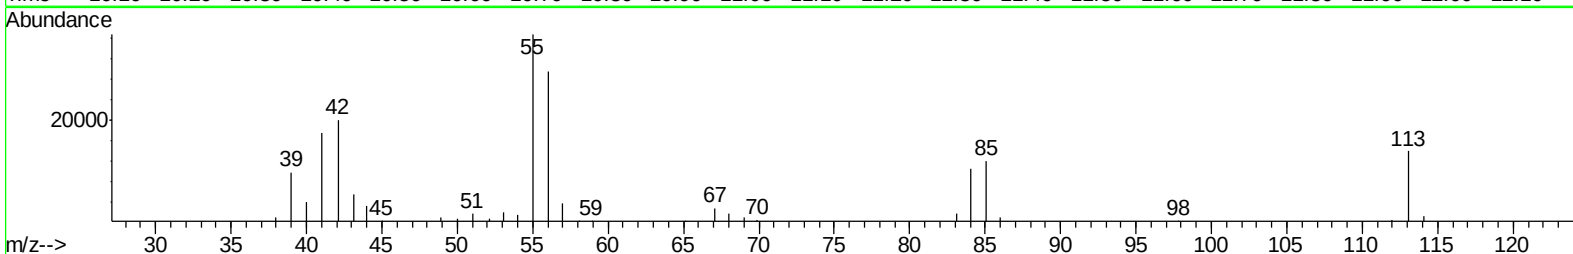


Data File : BN009709.D
Acq On : 11 Feb 2020 18:07
Operator : CG/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 12 00:56:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 00:52:44 2020
Response via : Initial Calibration

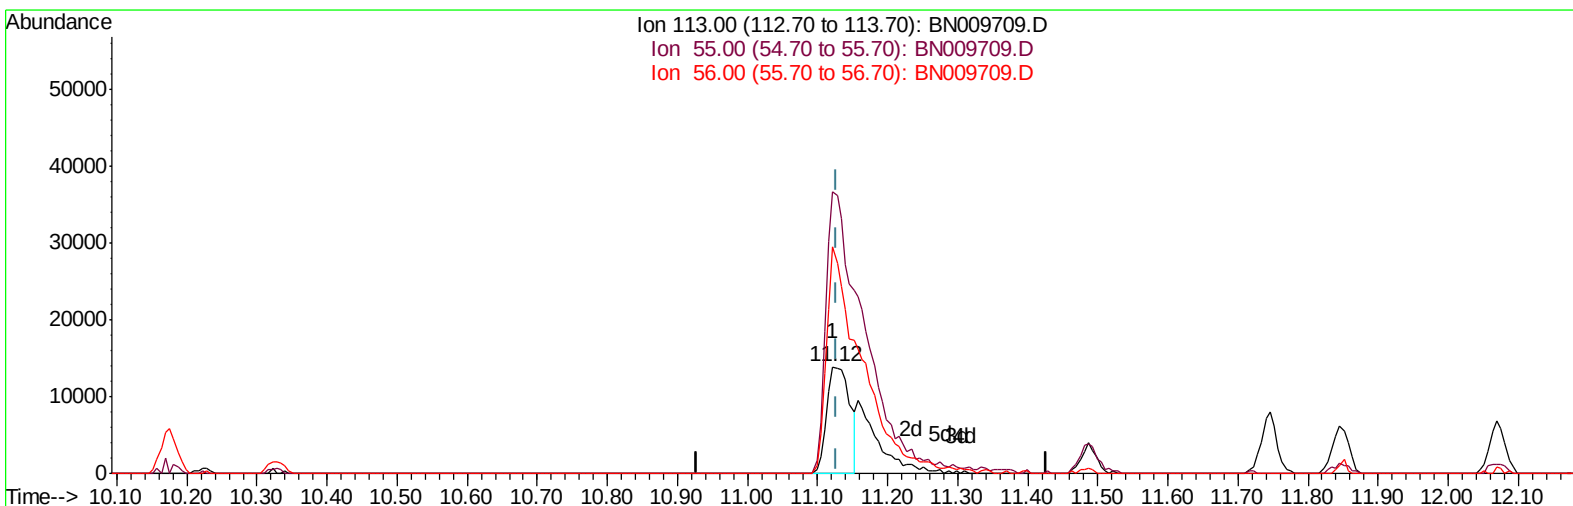

TIC: BN009709.D

(32) Caprolactam

11.122min (-0.006) 11.17ng/ul

response 31554

Ion	Exp%	Act%
113.00	100	100
55.00	258.80	263.70
56.00	199.10	211.62
0.00	0.00	0.00