

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029660.D
 Acq On : 10 Feb 2024 23:38
 Operator : MA/JU
 Sample : PB158928BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK928

Quant Time: Feb 11 23:23:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	7903	0.400	ng/ul	0.00
4) Naphthalene-d8	10.678	136	22355	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.520	164	10079	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.272	188	18151	0.400	ng/ul	0.00
17) Chrysene-d12	21.473	240	12085	0.400	ng/ul	0.00
23) Perylene-d12	23.840	264	14828	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	50559	5.131	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.273	152	7728	0.272	ng/ul	0.00
18) Fluoranthene-d10	19.309	212	10758	0.271	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.520	166	2234	0.057	ng/ul#	14
20) Pyrene	19.671	202	1892	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.688	252	3876	0.074	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
Data File : BN029660.D
Acq On : 10 Feb 2024 23:38
Operator : MA/JU
Sample : PB158928BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK928

Quant Time: Feb 11 23:23:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration




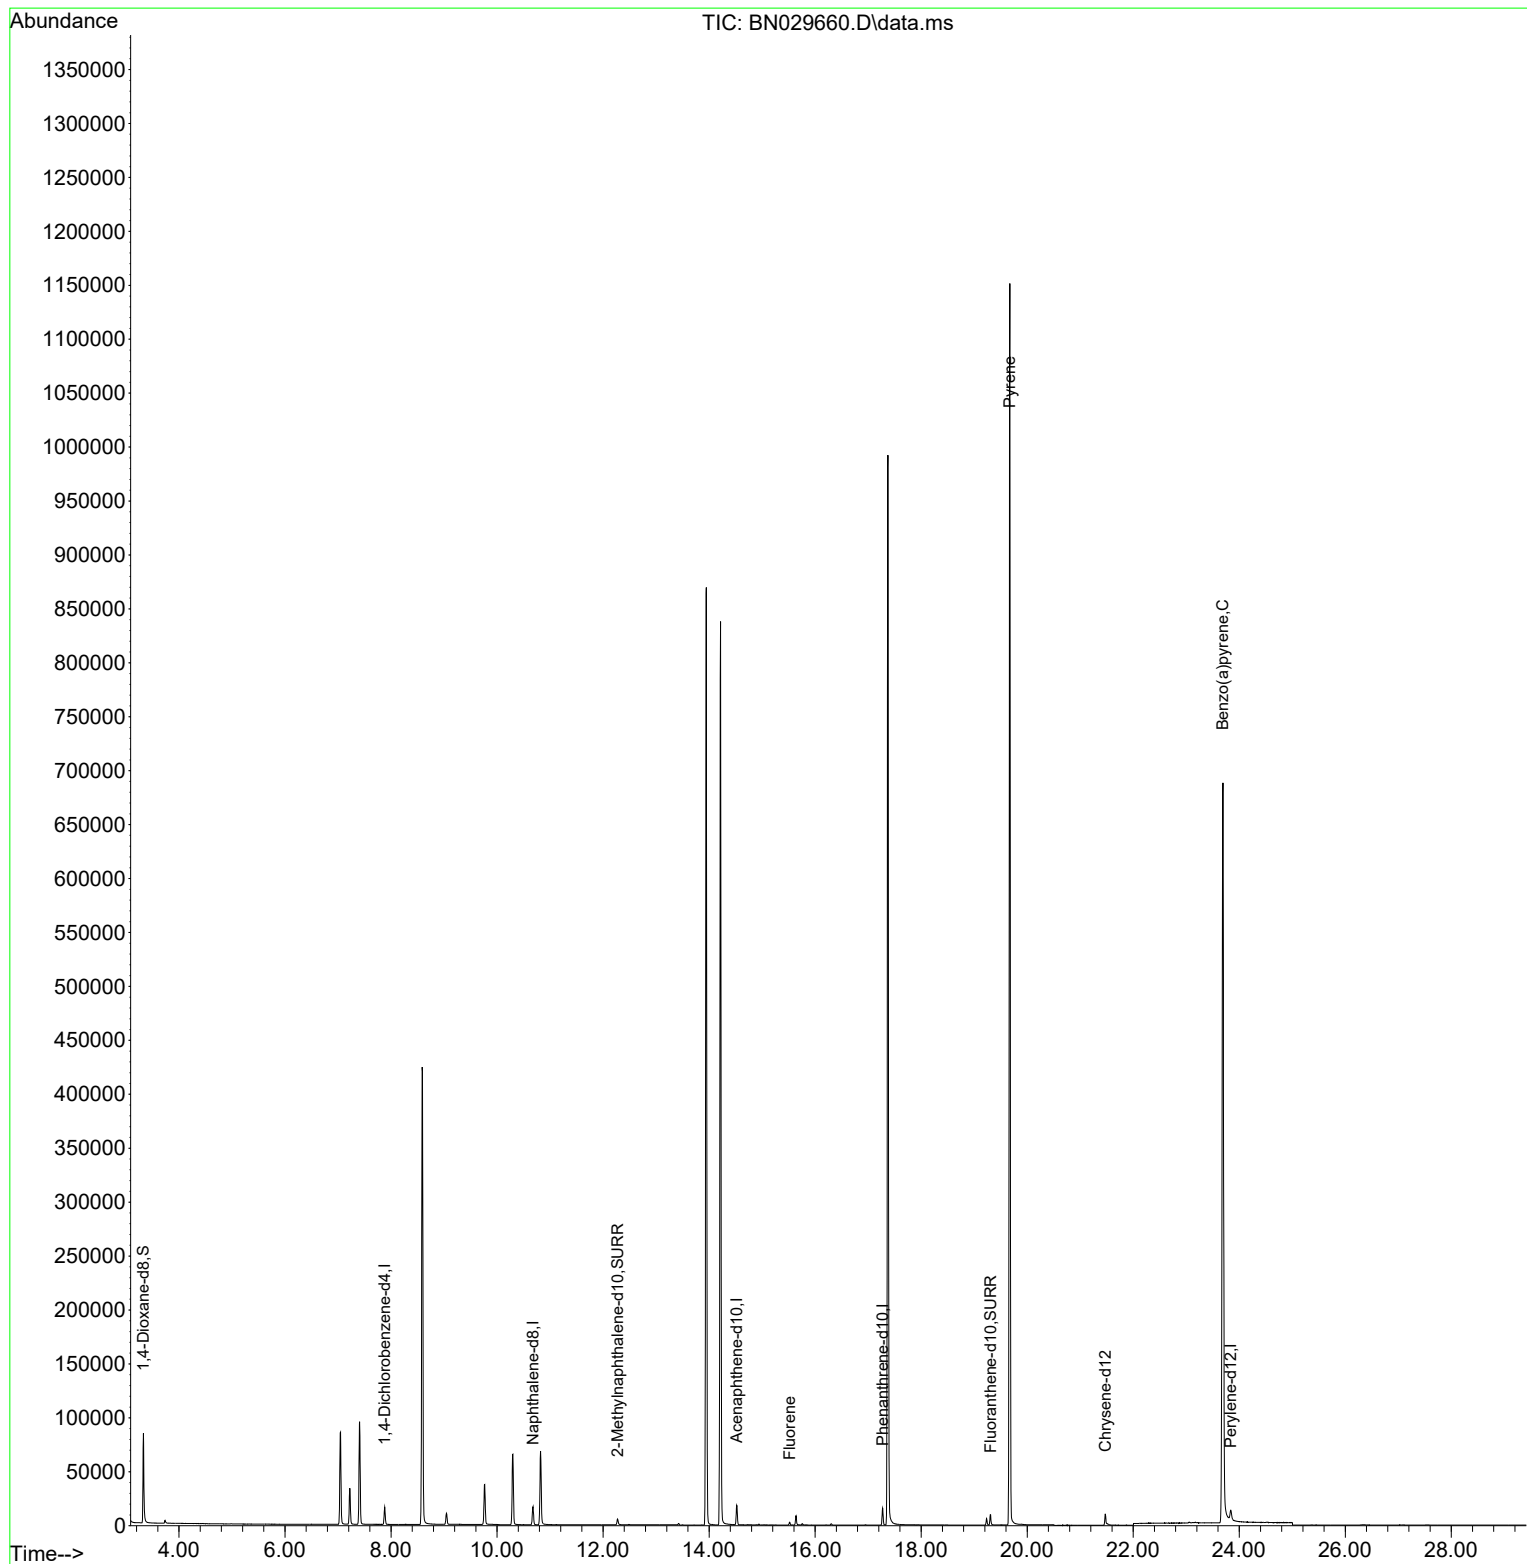


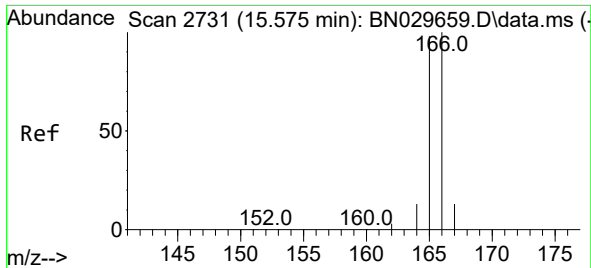

#12
Fluorene
Concen: 0.057 ng/ul
RT: 15.520 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN029660.D
Acq: 10 Feb 2024 23:38




Instrument :
BNA_N
ClientSampleId :
SBLK928


Tgt Ion:166 Resp: 2234
Ion Ratio Lower Upper
166 100
165 8.4 78.6 117.8#
167 36.7 11.5 17.3#

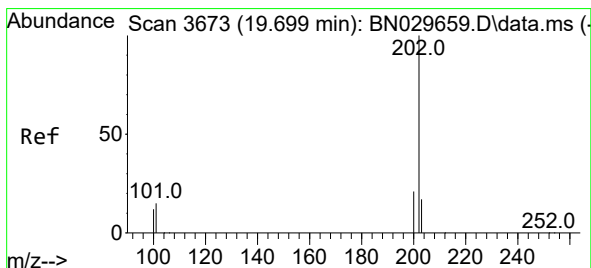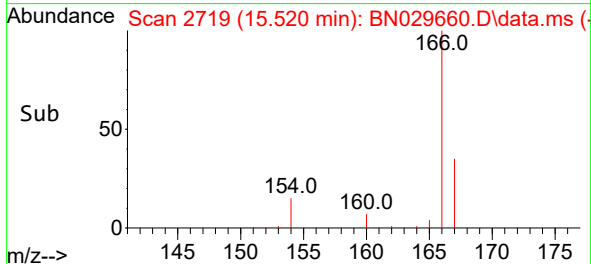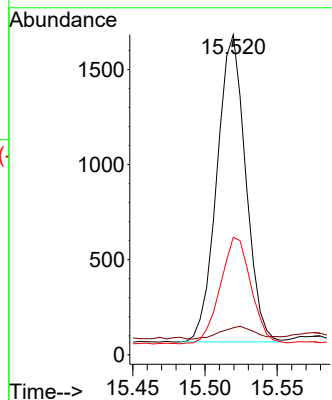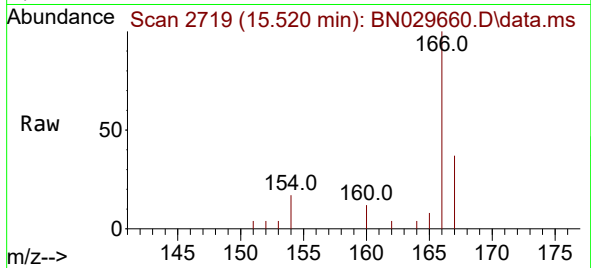

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.671 min Scan# 3667
Delta R.T. -0.028 min
Lab File: BN029660.D
Acq: 10 Feb 2024 23:38

Tgt Ion:202 Resp: 1892
Ion Ratio Lower Upper
202 100
101 194.7 12.5 18.7#
100 1450.3 10.0 15.0#

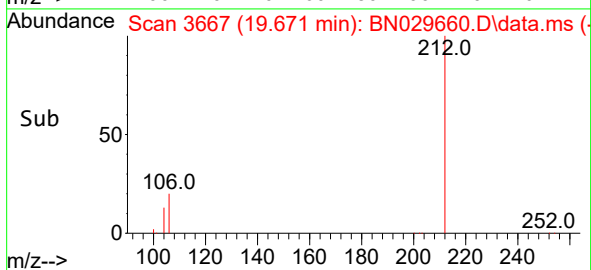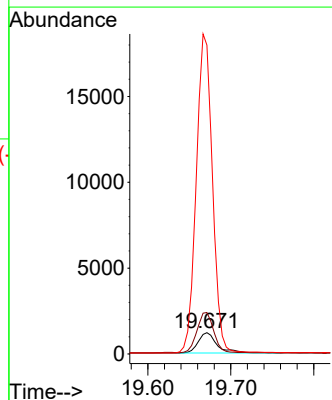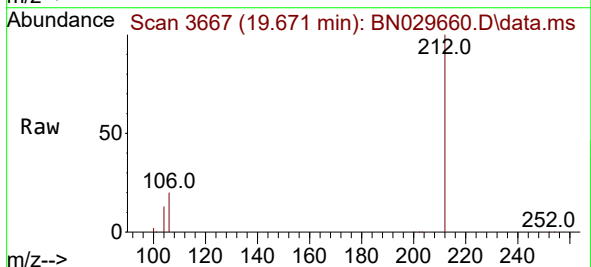

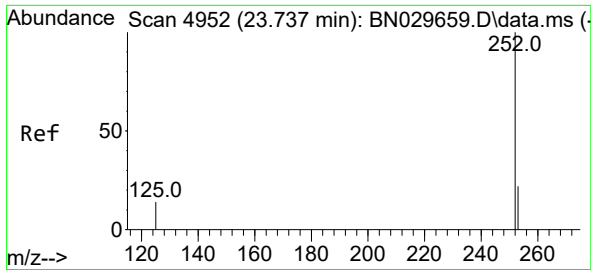

#26

Benzo(a)pyrene

Concen: 0.074 ng/ul

RT: 23.688 min Scan# 49

Delta R.T. -0.048 min

Lab File: BN029660.D


Acq: 10 Feb 2024 23:38

Instrument :

BNA_N

ClientSampleId :

SBLK928

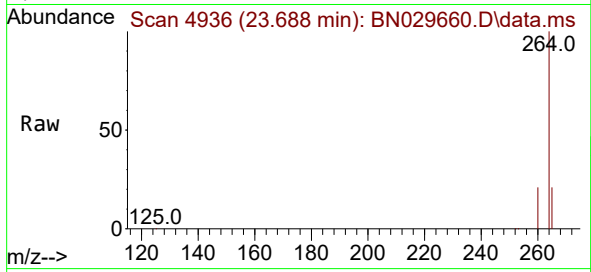

Tgt Ion:252 Resp: 3876

Ion Ratio Lower Upper

252 100

253 59.6 25.4 38.0#

125 39.6 16.0 24.0#

