

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029661.D
 Acq On : 11 Feb 2024 00:14
 Operator : MA/JU
 Sample : PB158930BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK930

Quant Time: Feb 11 23:23:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	5723	0.400	ng/ul	0.00
4) Naphthalene-d8	10.678	136	15878	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.520	164	7178	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.272	188	13270	0.400	ng/ul	0.00
17) Chrysene-d12	21.473	240	9152	0.400	ng/ul	0.00
23) Perylene-d12	23.840	264	11835	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	48397	6.782	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.272	152	7117	0.352	ng/ul	0.00
18) Fluoranthene-d10	19.304	212	10388	0.345	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.520	166	2113	0.076	ng/ul#	15
20) Pyrene	19.671	202	1838	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.691	252	3773	0.090	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
Data File : BN029661.D
Acq On : 11 Feb 2024 00:14
Operator : MA/JU
Sample : PB158930BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK930

Quant Time: Feb 11 23:23:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration

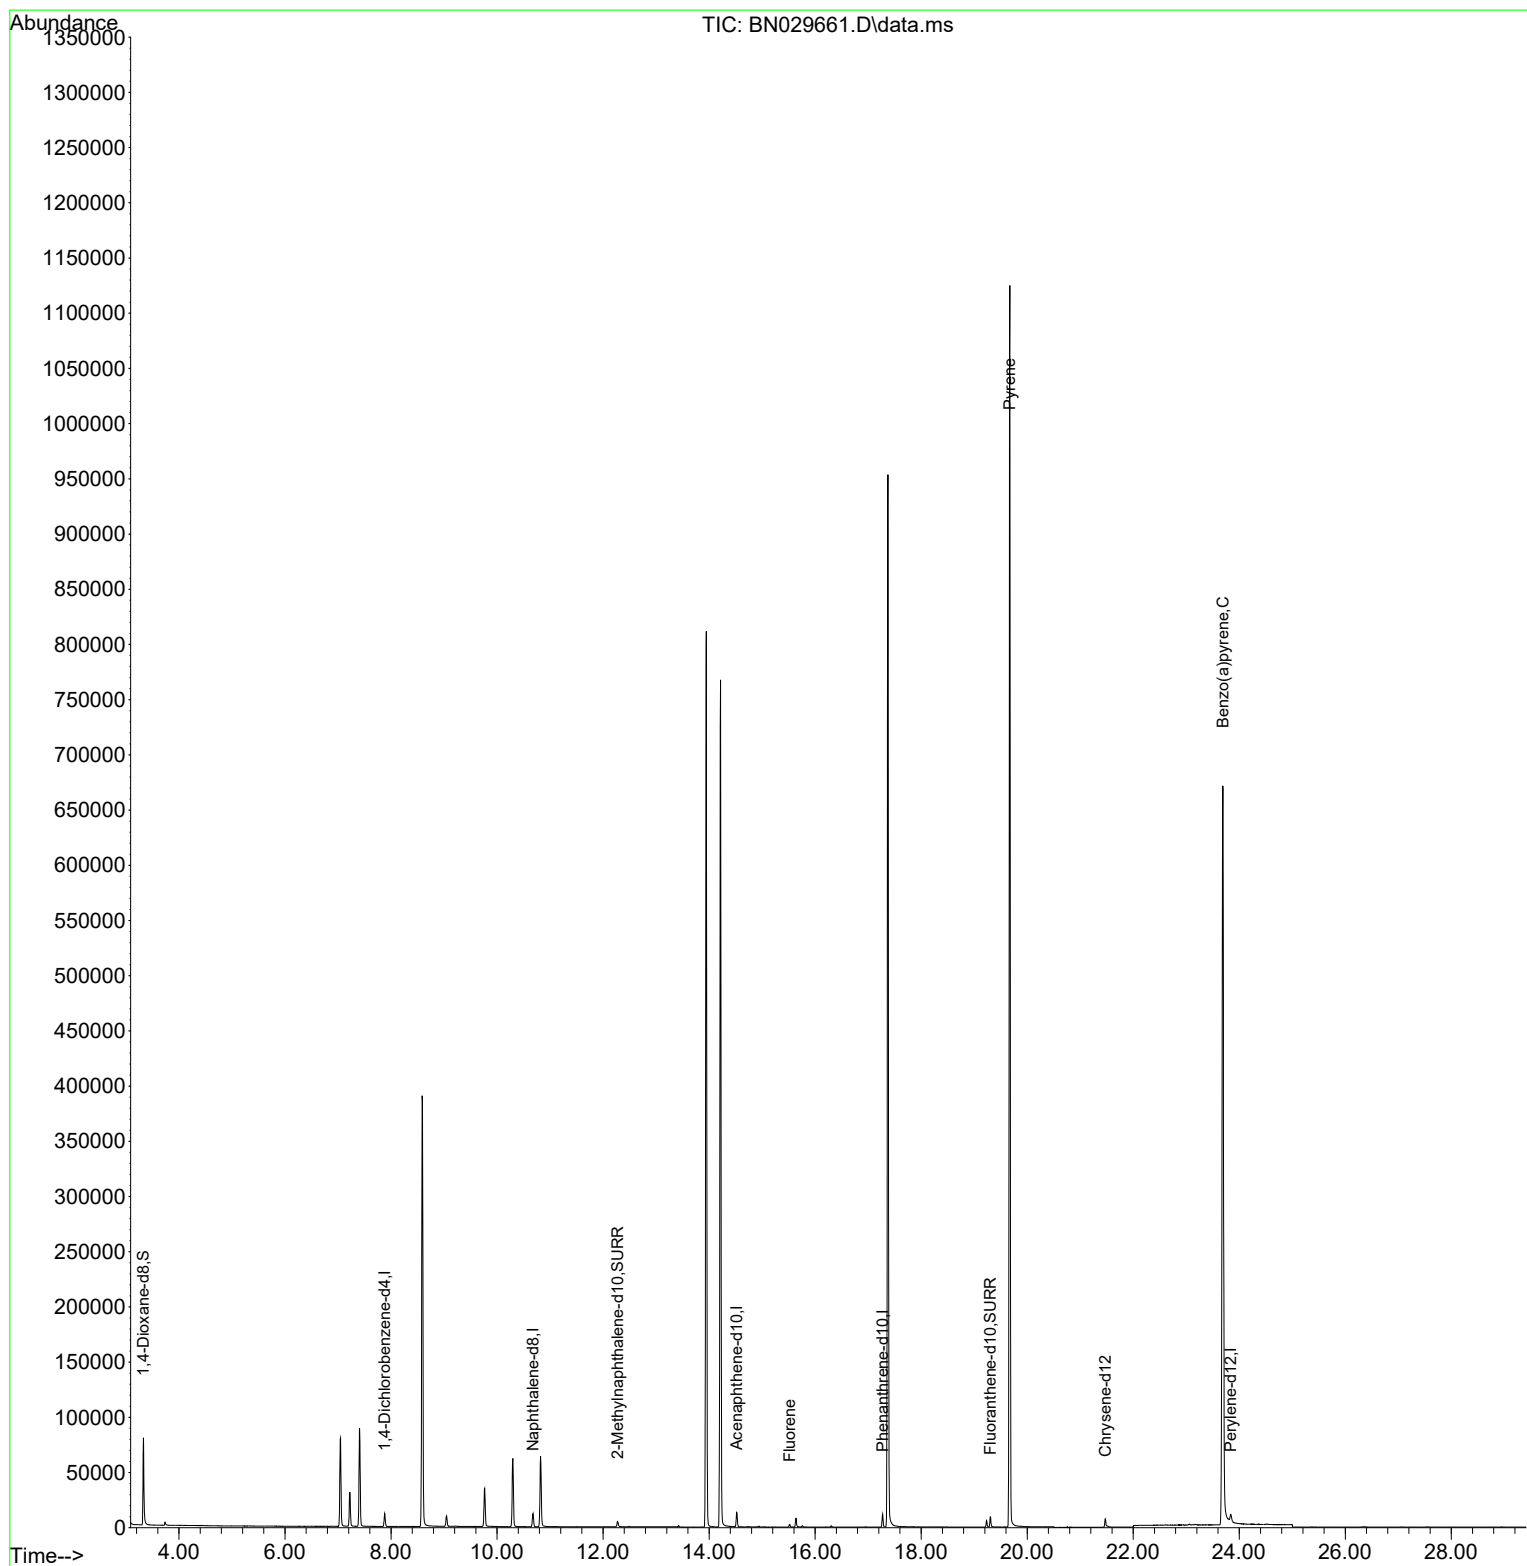

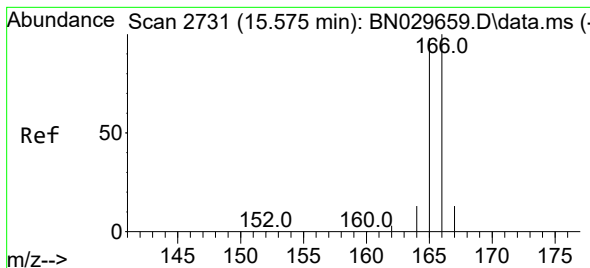

#12

Fluorene

Concen: 0.076 ng/ul

RT: 15.520 min Scan# 2113

Delta R.T. -0.056 min

Lab File: BN029661.D

Acq: 11 Feb 2024 00:14

Instrument :

BNA_N

ClientSampleId :

SBLK930





Tgt Ion:166 Resp: 2113

Ion Ratio Lower Upper

166 100

165 9.9 78.6 117.8#

167 37.3 11.5 17.3#

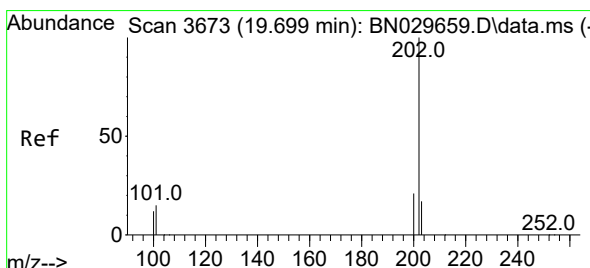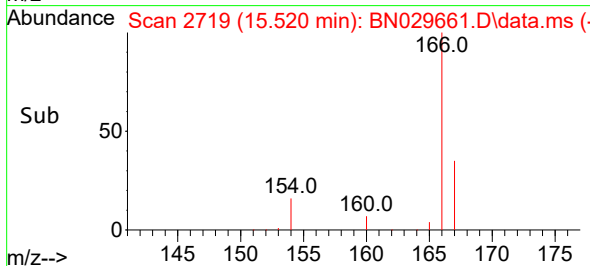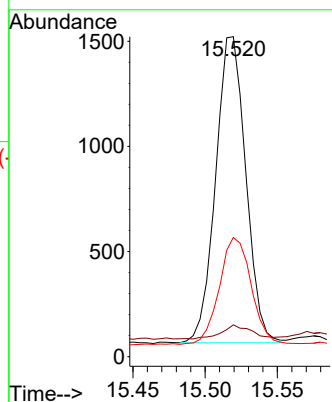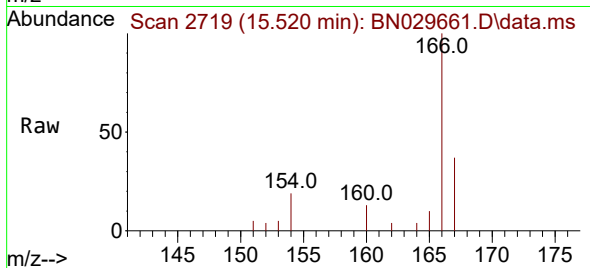

#20

Pyrene

Concen: 0.043 ng/ul

RT: 19.671 min Scan# 3667

Delta R.T. -0.028 min

Lab File: BN029661.D

Acq: 11 Feb 2024 00:14




Tgt Ion:202 Resp: 1838


Ion Ratio Lower Upper

202 100

101 196.8 12.5 18.7#


100 1424.3 10.0 15.0#

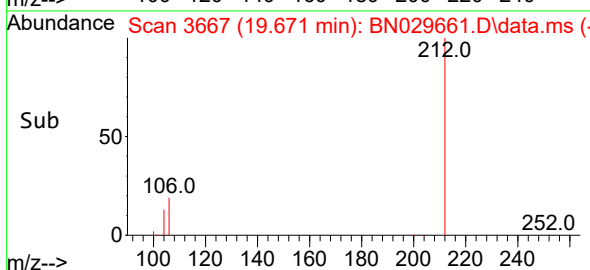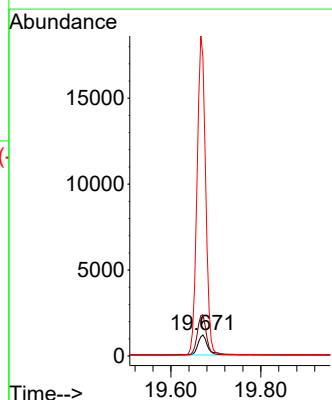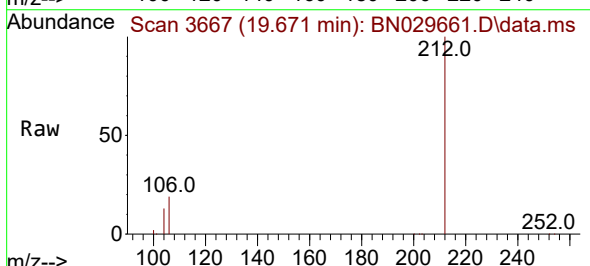

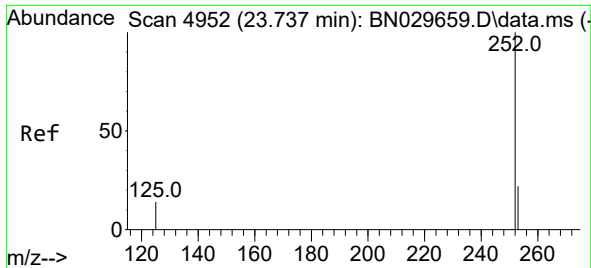

#26
Benzo(a)pyrene
Concen: 0.090 ng/ul
RT: 23.691 min Scan# 4937
Delta R.T. -0.046 min
Lab File: BN029661.D
Acq: 11 Feb 2024 00:14

Instrument :
BNA_N
ClientSampleId :
SBLK930

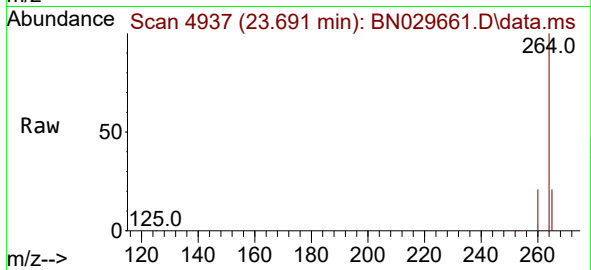

Tgt Ion:252 Resp: 3773
Ion Ratio Lower Upper
252 100
253 58.9 25.4 38.0#
125 37.5 16.0 24.0#

