

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029677.D
 Acq On : 11 Feb 2024 10:29
 Operator : MA/JU
 Sample : PB158922BL
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK922

Quant Time: Feb 11 23:26:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	6265	0.400	ng/ul	0.00
4) Naphthalene-d8	10.678	136	17624	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.520	164	8040	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.272	188	13884	0.400	ng/ul	0.00
17) Chrysene-d12	21.473	240	8643	0.400	ng/ul	0.00
23) Perylene-d12	23.840	264	11749	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	47286	6.053	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.273	152	6885	0.307	ng/ul	0.00
18) Fluoranthene-d10	19.304	212	9056	0.319	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.515	166	2063	0.066	ng/ul#	16
20) Pyrene	19.671	202	1507	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.691	252	3337	0.080	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
Data File : BN029677.D
Acq On : 11 Feb 2024 10:29
Operator : MA/JU
Sample : PB158922BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK922

Quant Time: Feb 11 23:26:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration




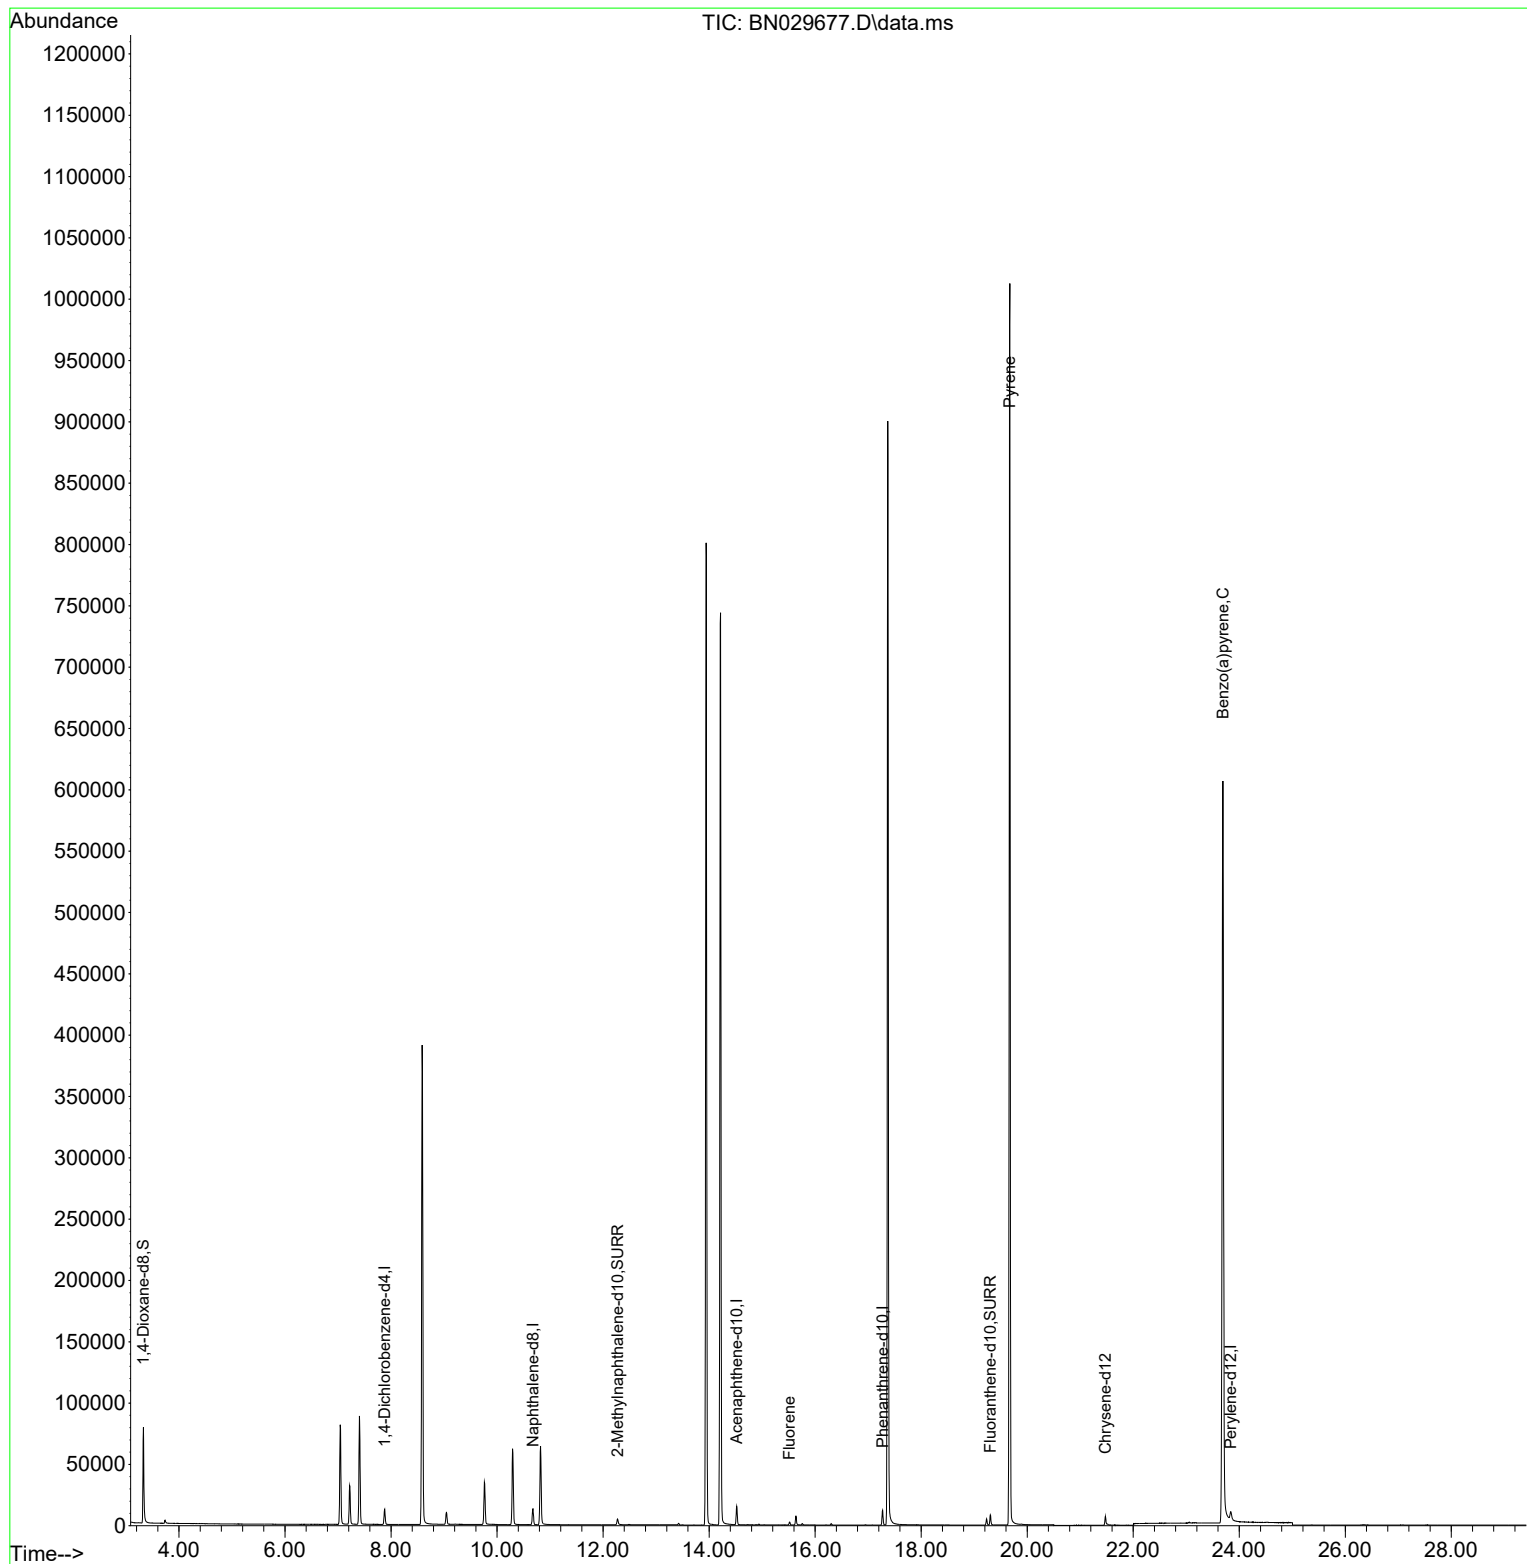


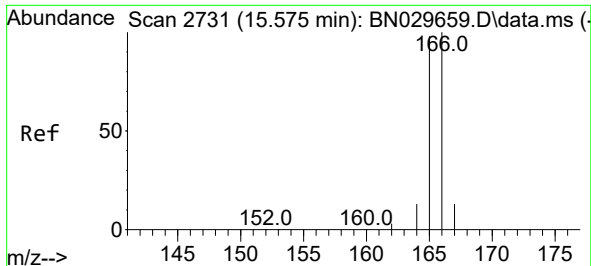

#12
Fluorene
Concen: 0.066 ng/ul
RT: 15.515 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN029677.D
Acq: 11 Feb 2024 10:29




Instrument :
BNA_N
ClientSampleId :
SBLK922


Tgt Ion:166 Resp: 2063
Ion Ratio Lower Upper
166 100
165 8.9 78.6 117.8#
167 32.9 11.5 17.3#

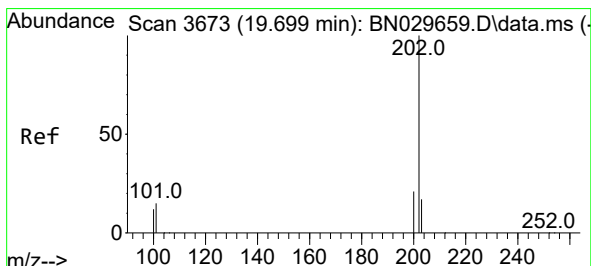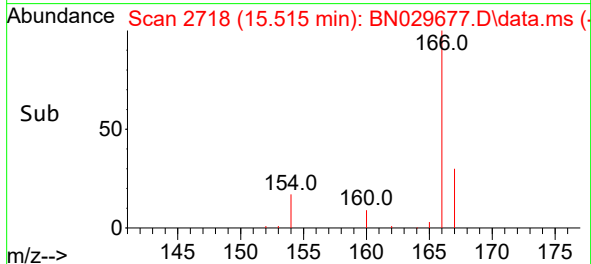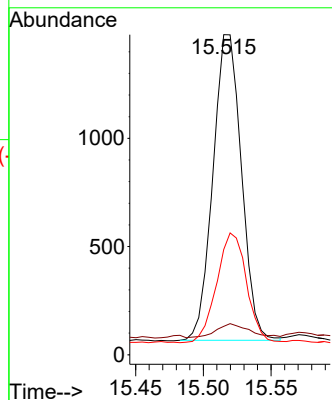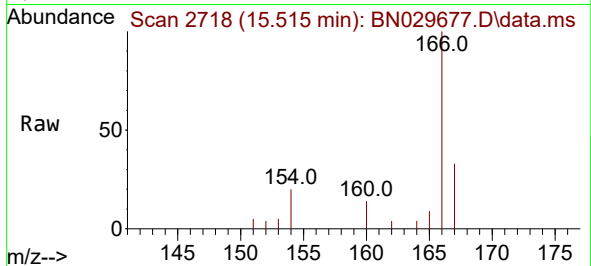

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.671 min Scan# 3667
Delta R.T. -0.028 min
Lab File: BN029677.D
Acq: 11 Feb 2024 10:29

Tgt Ion:202 Resp: 1507
Ion Ratio Lower Upper
202 100
101 195.7 12.5 18.7#
100 1421.5 10.0 15.0#

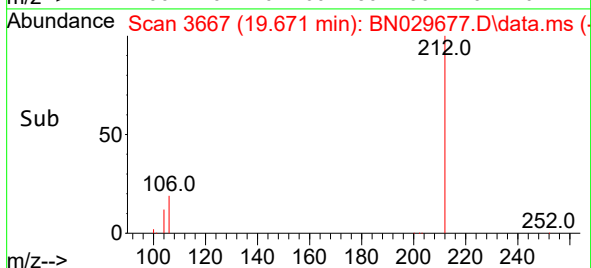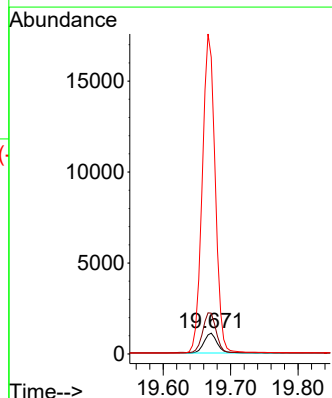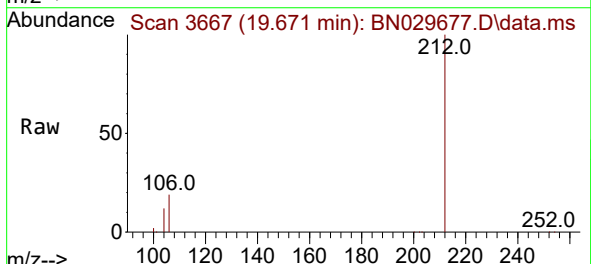

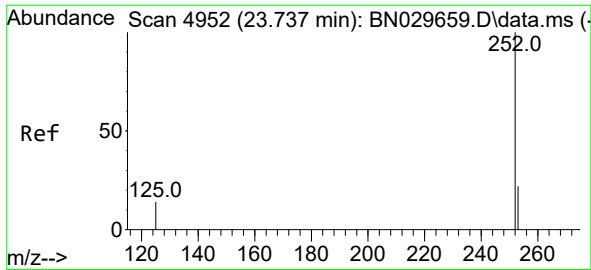

#26

Benzo(a)pyrene

Concen: 0.080 ng/ul

RT: 23.691 min Scan# 4937

Delta R.T. -0.045 min

Lab File: BN029677.D


Acq: 11 Feb 2024 10:29

Instrument :

BNA_N

ClientSampleId :

SBLK922

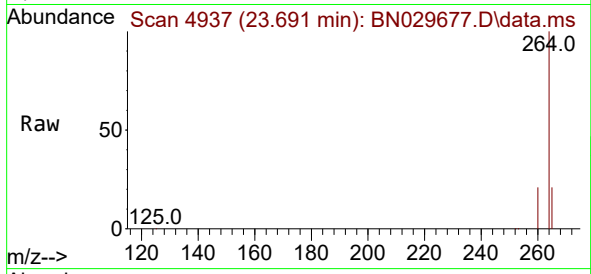

Tgt Ion:252 Resp: 3337

Ion Ratio Lower Upper

252 100

253 58.8 25.4 38.0#

125 39.4 16.0 24.0#

