

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029678.D
 Acq On : 11 Feb 2024 11:05
 Operator : MA/JU
 Sample : PB158926BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK926

Quant Time: Feb 11 23:26:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	5871	0.400	ng/ul	0.00
4) Naphthalene-d8	10.678	136	16358	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.520	164	7351	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.272	188	12935	0.400	ng/ul	0.00
17) Chrysene-d12	21.474	240	8211	0.400	ng/ul	0.00
23) Perylene-d12	23.842	264	11552	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	52842	7.218	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.272	152	7673	0.369	ng/ul	0.00
18) Fluoranthene-d10	19.304	212	10355	0.384	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.515	166	2243	0.079	ng/ul#	15
20) Pyrene	19.671	202	1718	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.690	252	3900	0.095	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
Data File : BN029678.D
Acq On : 11 Feb 2024 11:05
Operator : MA/JU
Sample : PB158926BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK926


Quant Time: Feb 11 23:26:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration

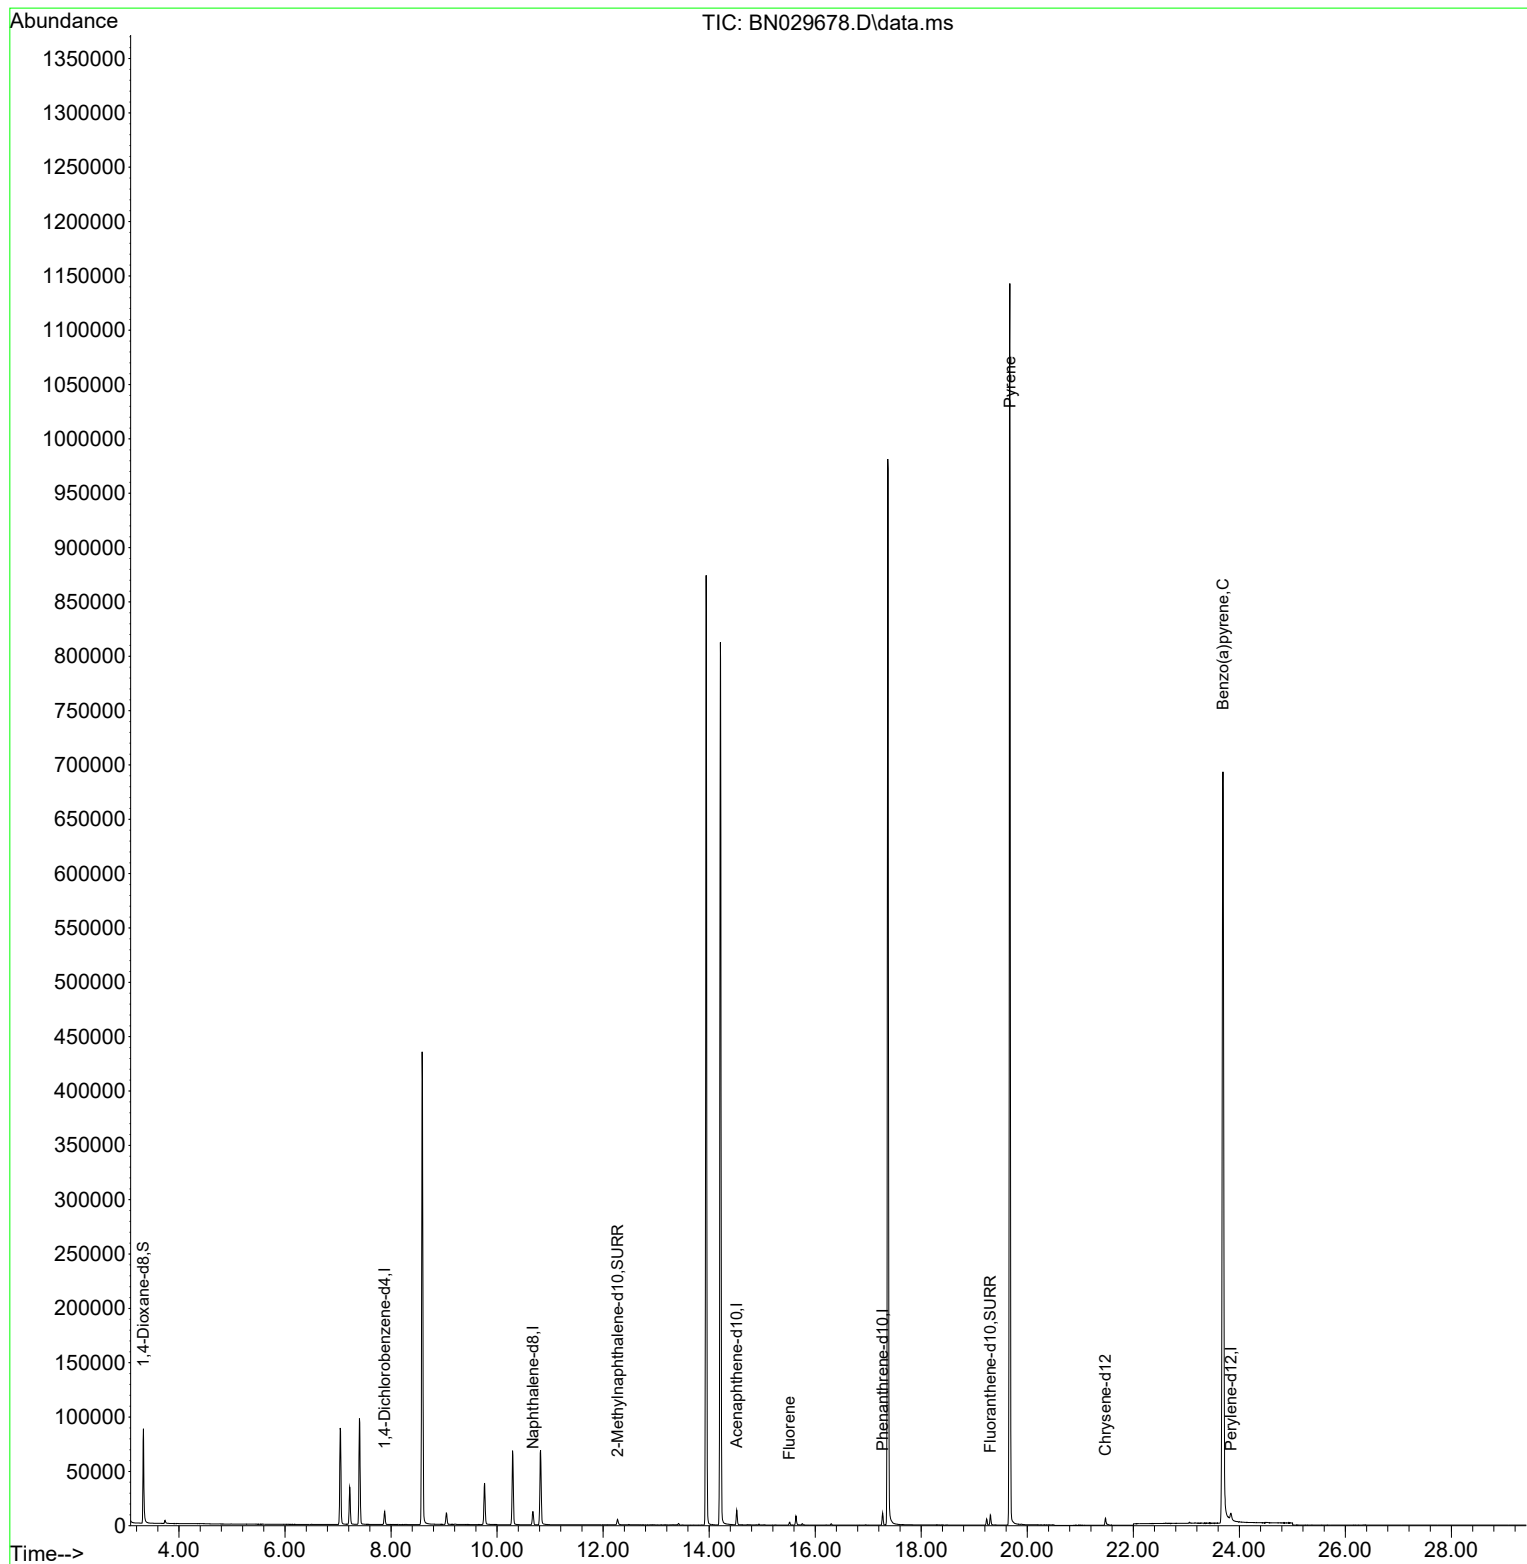



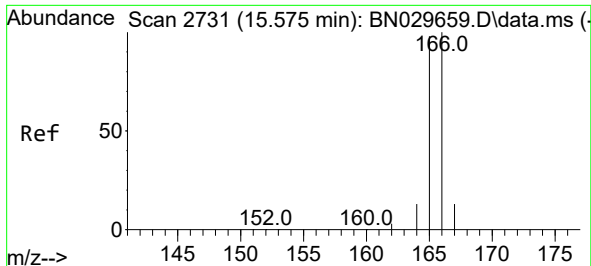


#12
Fluorene
Concen: 0.079 ng/ul
RT: 15.515 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN029678.D
Acq: 11 Feb 2024 11:05

Instrument :
BNA_N
ClientSampleId :
SBLK926



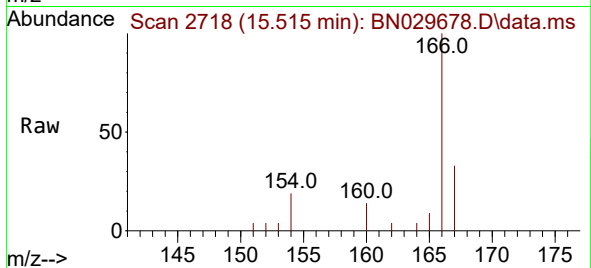



Tgt Ion:166 Resp: 2243
Ion Ratio Lower Upper
166 100
165 8.7 78.6 117.8#
167 33.1 11.5 17.3#

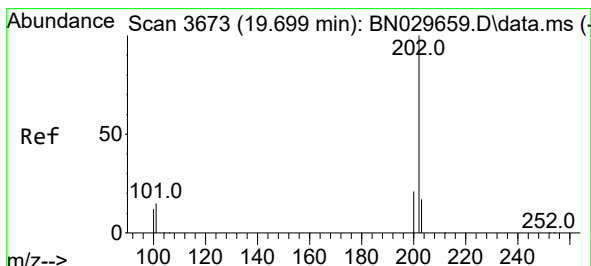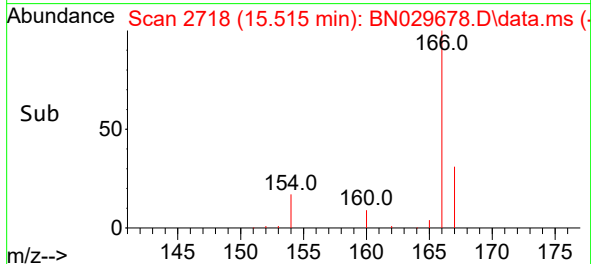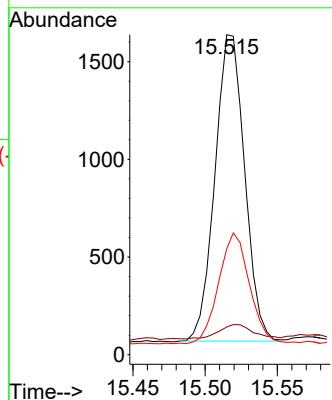

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.671 min Scan# 3667
Delta R.T. -0.028 min
Lab File: BN029678.D
Acq: 11 Feb 2024 11:05

Tgt Ion:202 Resp: 1718
Ion Ratio Lower Upper
202 100
101 199.0 12.5 18.7#
100 1456.5 10.0 15.0#

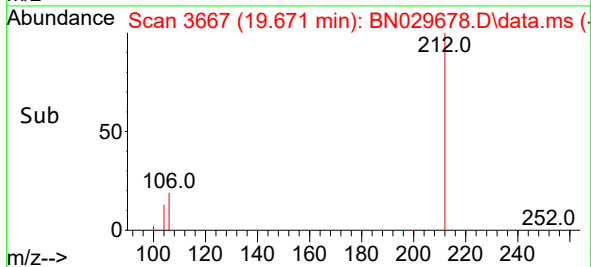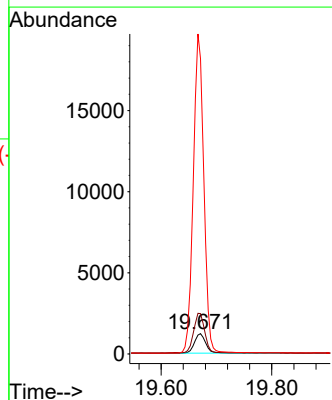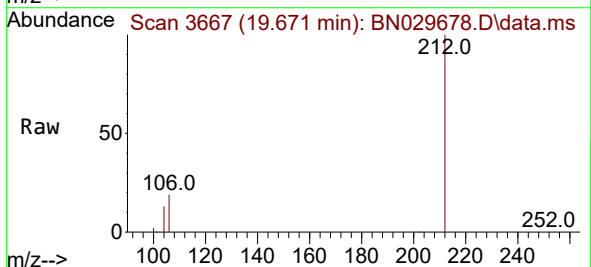

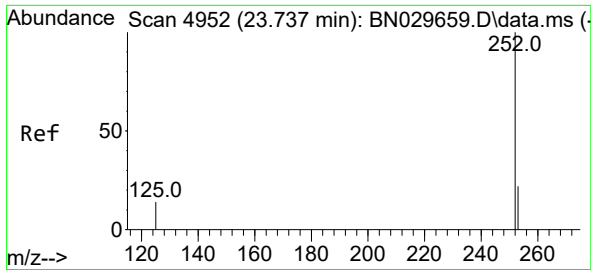

#26

Benzo(a)pyrene

Concen: 0.095 ng/ul

RT: 23.690 min Scan# 4936

Delta R.T. -0.047 min

Lab File: BN029678.D


Acq: 11 Feb 2024 11:05

Instrument :

BNA_N

ClientSampleId :

SBLK926

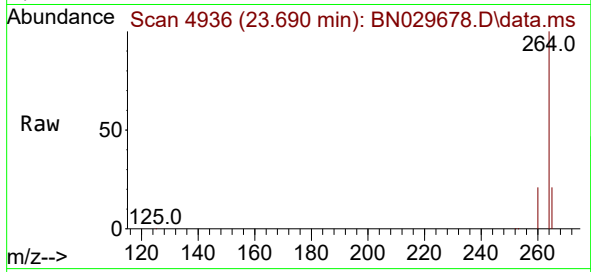

Tgt Ion:252 Resp: 3900

Ion Ratio Lower Upper

252 100

253 53.3 25.4 38.0#

125 38.3 16.0 24.0#

