

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029680.D
 Acq On : 11 Feb 2024 12:18
 Operator : MA/JU
 Sample : P1398-09
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG3

Quant Time: Feb 11 23:26:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	6158	0.400	ng/ul	0.00
4) Naphthalene-d8	10.672	136	17398	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.520	164	7967	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.272	188	13945	0.400	ng/ul	0.00
17) Chrysene-d12	21.473	240	8484	0.400	ng/ul	0.00
23) Perylene-d12	23.840	264	11514	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	36404	4.741	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.273	152	9473	0.428	ng/ul	0.00
18) Fluoranthene-d10	19.304	212	12836	0.460	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.520	166	2773	0.090	ng/ul#	14
20) Pyrene	19.671	202	2028	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.691	252	4330	0.106	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
Data File : BN029680.D
Acq On : 11 Feb 2024 12:18
Operator : MA/JU
Sample : P1398-09
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG3

Quant Time: Feb 11 23:26:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration




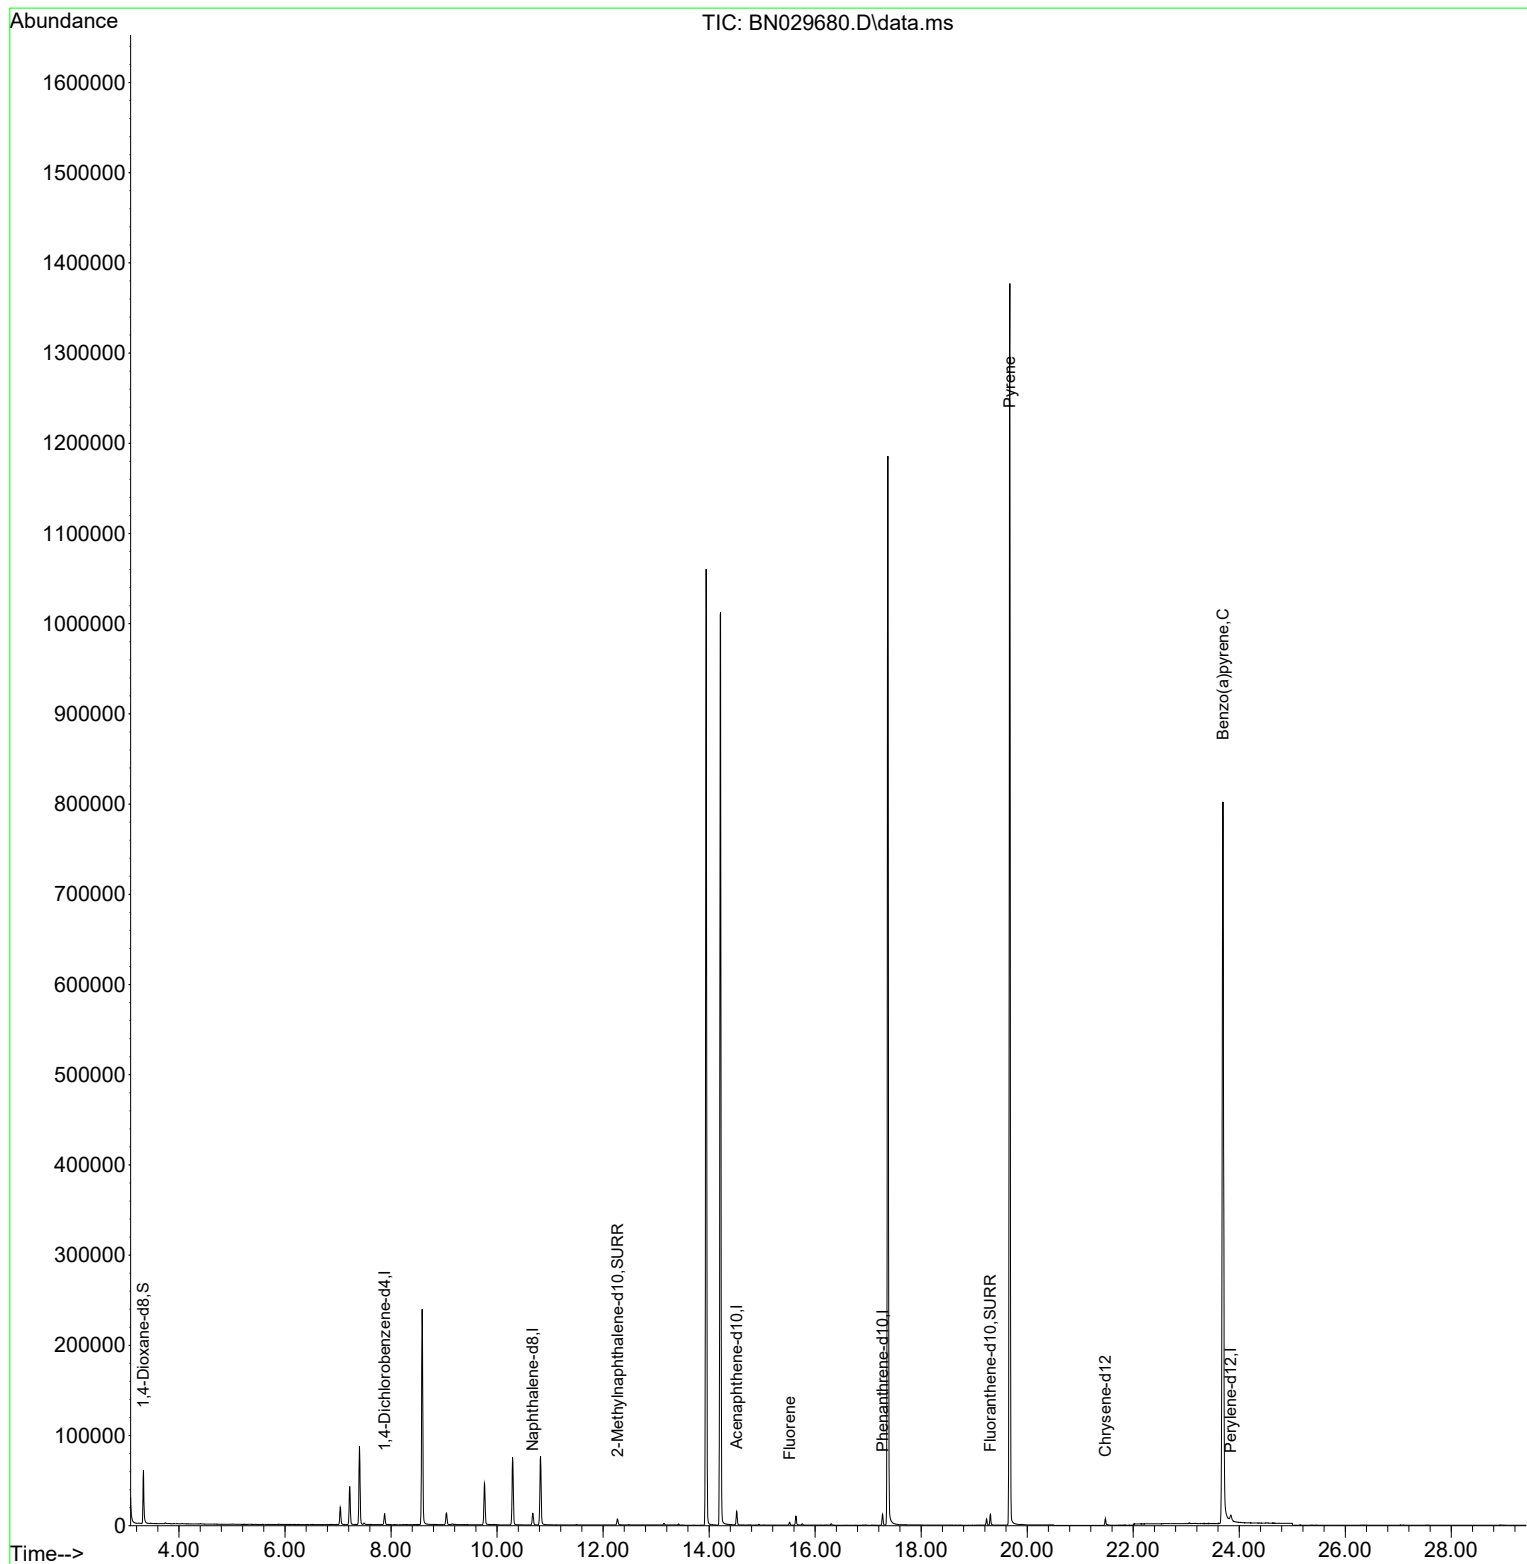


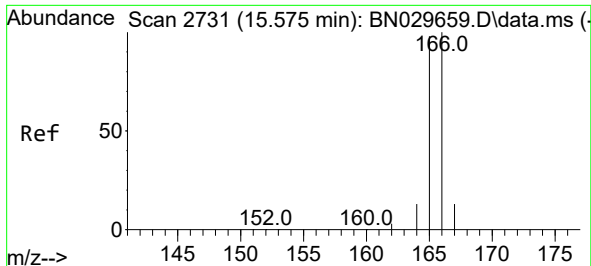

#12
Fluorene
Concen: 0.090 ng/ul
RT: 15.520 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN029680.D
Acq: 11 Feb 2024 12:18




Instrument :
BNA_N
ClientSampleId :
C0AG3


Tgt Ion:166 Resp: 2773
Ion Ratio Lower Upper
166 100
165 8.4 78.6 117.8#
167 36.0 11.5 17.3#

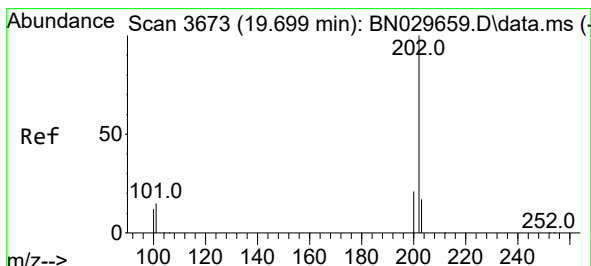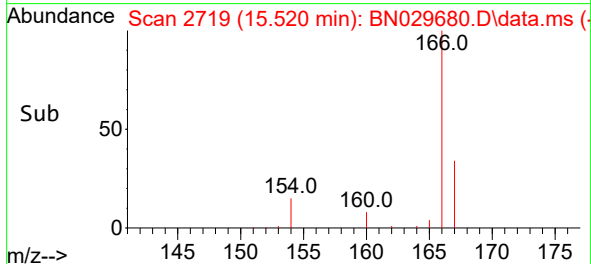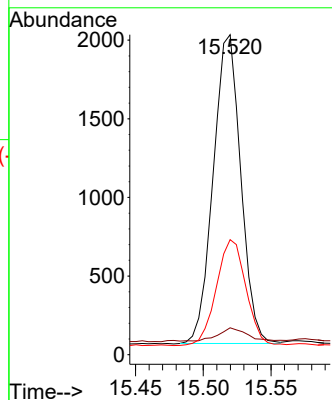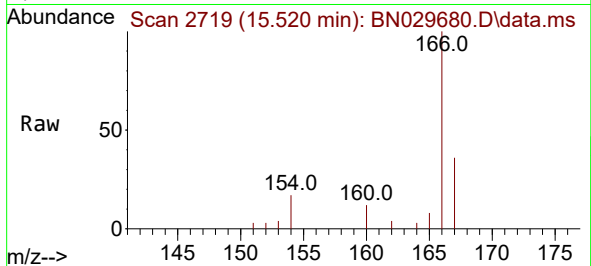

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.671 min Scan# 3667
Delta R.T. -0.028 min
Lab File: BN029680.D
Acq: 11 Feb 2024 12:18


Tgt Ion:202 Resp: 2028
Ion Ratio Lower Upper
202 100
101 196.1 12.5 18.7#
100 1458.7 10.0 15.0#

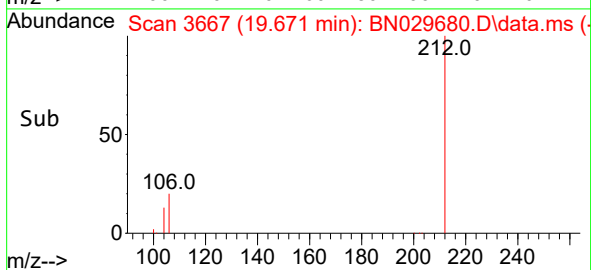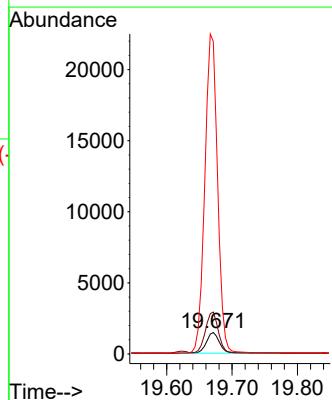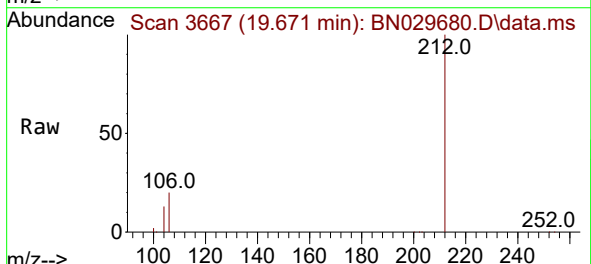

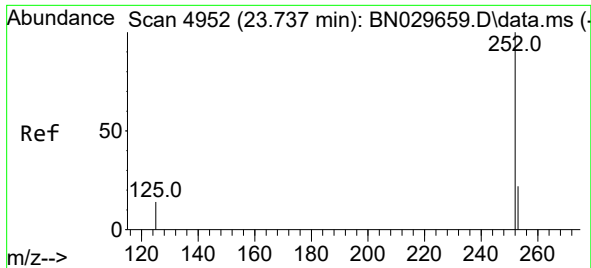

#26
Benzo(a)pyrene
Concen: 0.106 ng/ul
RT: 23.691 min Scan# 4937
Delta R.T. -0.045 min
Lab File: BN029680.D
Acq: 11 Feb 2024 12:18

Instrument :
BNA_N
ClientSampleId :
C0AG3

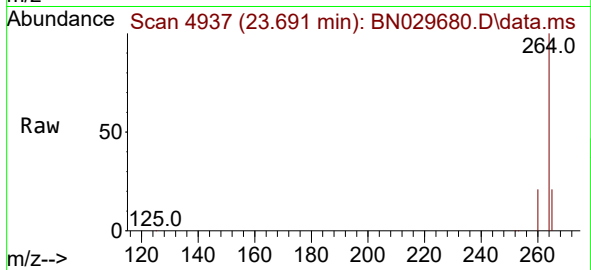

Tgt Ion:252 Resp: 4330
Ion Ratio Lower Upper
252 100
253 53.4 25.4 38.0#
125 37.9 16.0 24.0#

