

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029684.D
 Acq On : 11 Feb 2024 14:42
 Operator : MA/JU
 Sample : P1398-18
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH2

Quant Time: Feb 11 23:26:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	6672	0.400	ng/ul	0.00
4) Naphthalene-d8	10.672	136	19010	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.520	164	8687	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.272	188	15476	0.400	ng/ul	0.00
17) Chrysene-d12	21.474	240	9625	0.400	ng/ul	0.00
23) Perylene-d12	23.842	264	12488	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	37935	4.560	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.267	152	9376	0.388	ng/ul	0.00
18) Fluoranthene-d10	19.304	212	14629	0.462	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.515	166	2835	0.084	ng/ul#	14
20) Pyrene	19.671	202	2117	0.047	ng/ul#	1
26) Benzo(a)pyrene	23.690	252	4393	0.099	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
Data File : BN029684.D
Acq On : 11 Feb 2024 14:42
Operator : MA/JU
Sample : P1398-18
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH2


Quant Time: Feb 11 23:26:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration

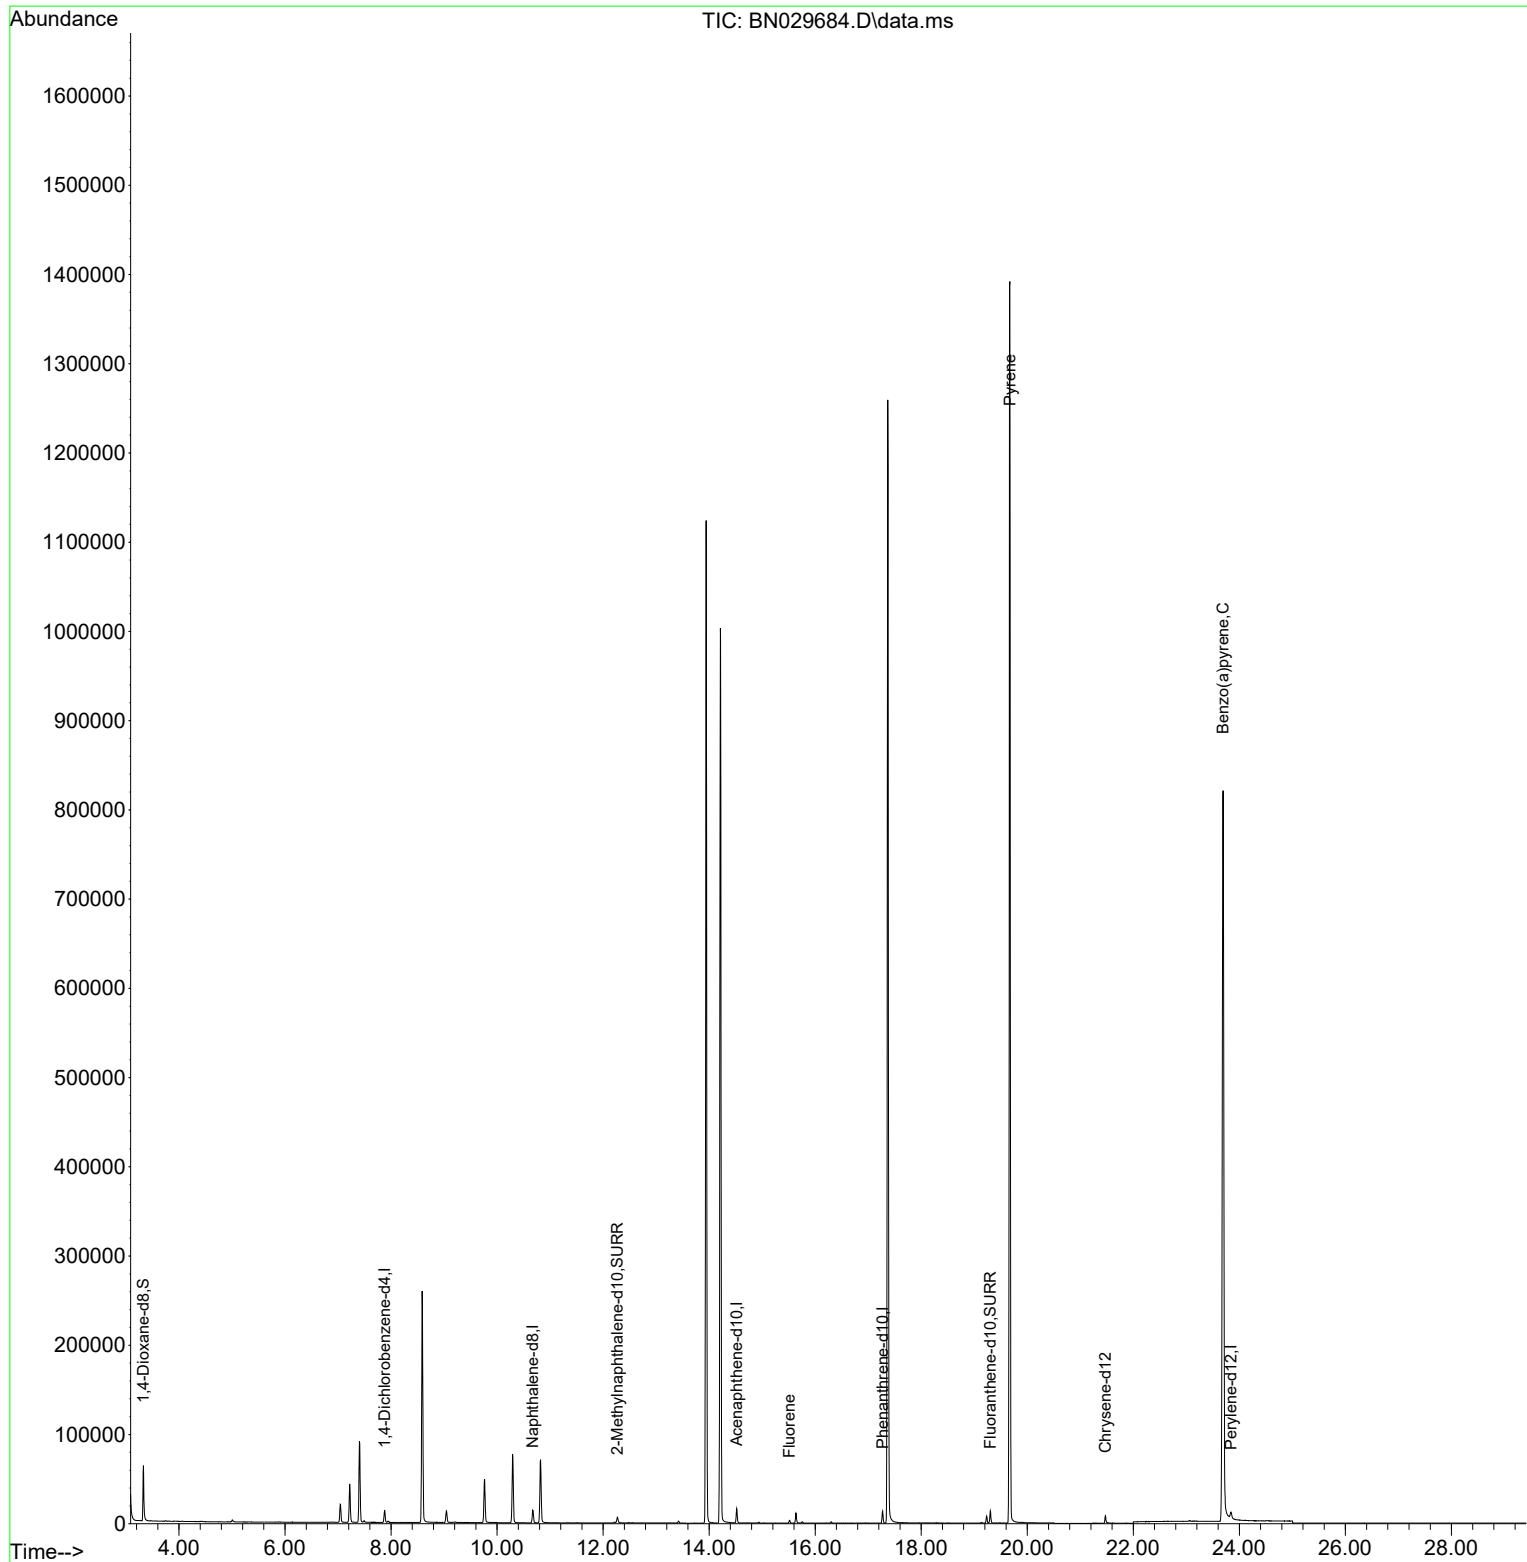



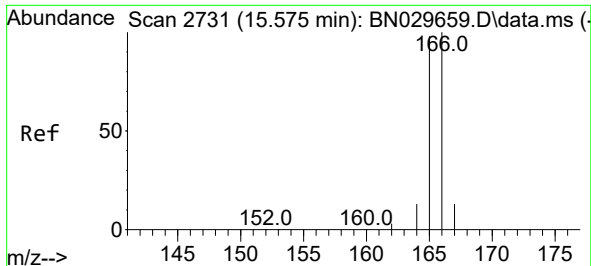


#12
Fluorene
Concen: 0.084 ng/ul
RT: 15.515 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN029684.D
Acq: 11 Feb 2024 14:42

Instrument :
BNA_N
ClientSampleId :
C0AH2



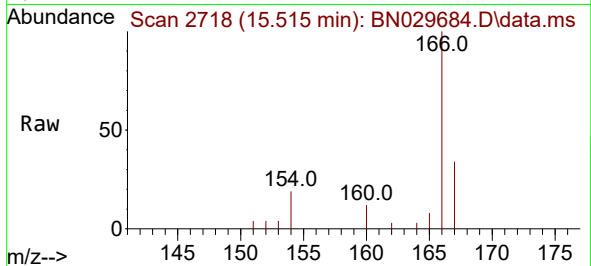



Tgt Ion:166 Resp: 2835
Ion Ratio Lower Upper
166 100
165 7.9 78.6 117.8#
167 34.0 11.5 17.3#

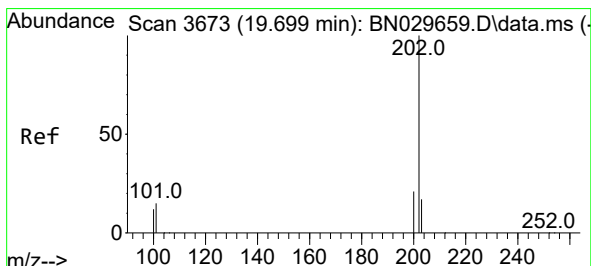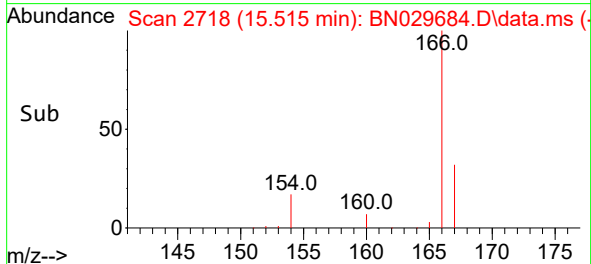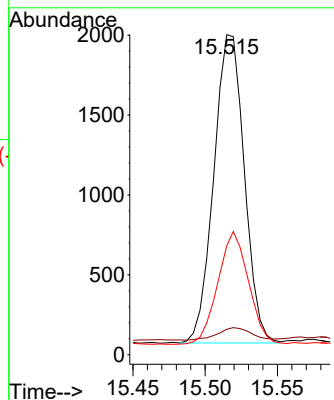

#20
Pyrene
Concen: 0.047 ng/ul
RT: 19.671 min Scan# 3667
Delta R.T. -0.028 min
Lab File: BN029684.D
Acq: 11 Feb 2024 14:42


Tgt Ion:202 Resp: 2117
Ion Ratio Lower Upper
202 100
101 186.0 12.5 18.7#
100 1334.5 10.0 15.0#

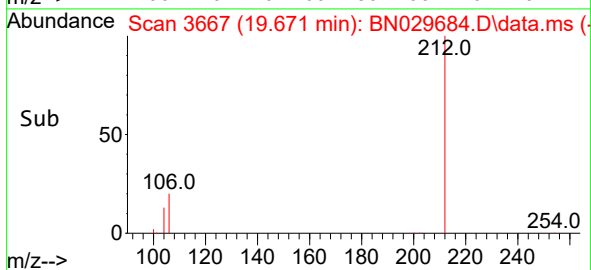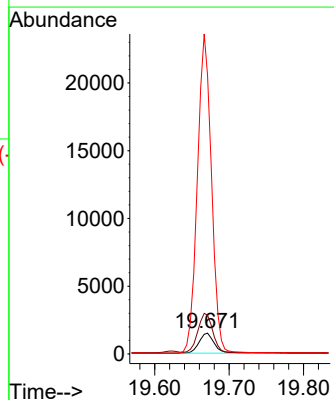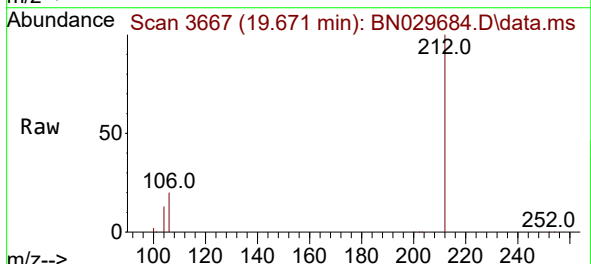

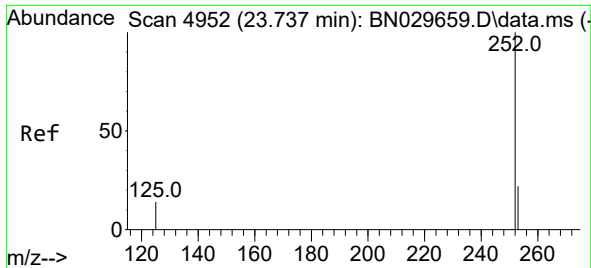

#26
Benzo(a)pyrene
Concen: 0.099 ng/ul
RT: 23.690 min Scan# 4936
Delta R.T. -0.047 min
Lab File: BN029684.D
Acq: 11 Feb 2024 14:42

Instrument :
BNA_N
ClientSampleId :
C0AH2

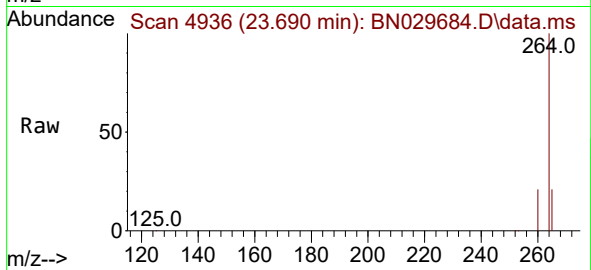

Tgt Ion:252 Resp: 4393
Ion Ratio Lower Upper
252 100
253 53.3 25.4 38.0#
125 38.4 16.0 24.0#

