

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029695.D
 Acq On : 11 Feb 2024 21:56
 Operator : MA/JU
 Sample : PB158924BL
 Misc :
 ALS Vial : 89 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK924

Quant Time: Feb 11 23:29:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	5240	0.400	ng/ul	0.00
4) Naphthalene-d8	10.672	136	14323	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.520	164	6340	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.272	188	11544	0.400	ng/ul	0.00
17) Chrysene-d12	21.471	240	7733	0.400	ng/ul	0.00
23) Perylene-d12	23.836	264	10155	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	45181	6.915	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.272	152	6123	0.336	ng/ul	0.00
18) Fluoranthene-d10	19.304	212	8866	0.349	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.515	166	1787	0.073	ng/ul#	16
20) Pyrene	19.671	202	1438	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.687	252	3313	0.092	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
Data File : BN029695.D
Acq On : 11 Feb 2024 21:56
Operator : MA/JU
Sample : PB158924BL
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK924

Quant Time: Feb 11 23:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration




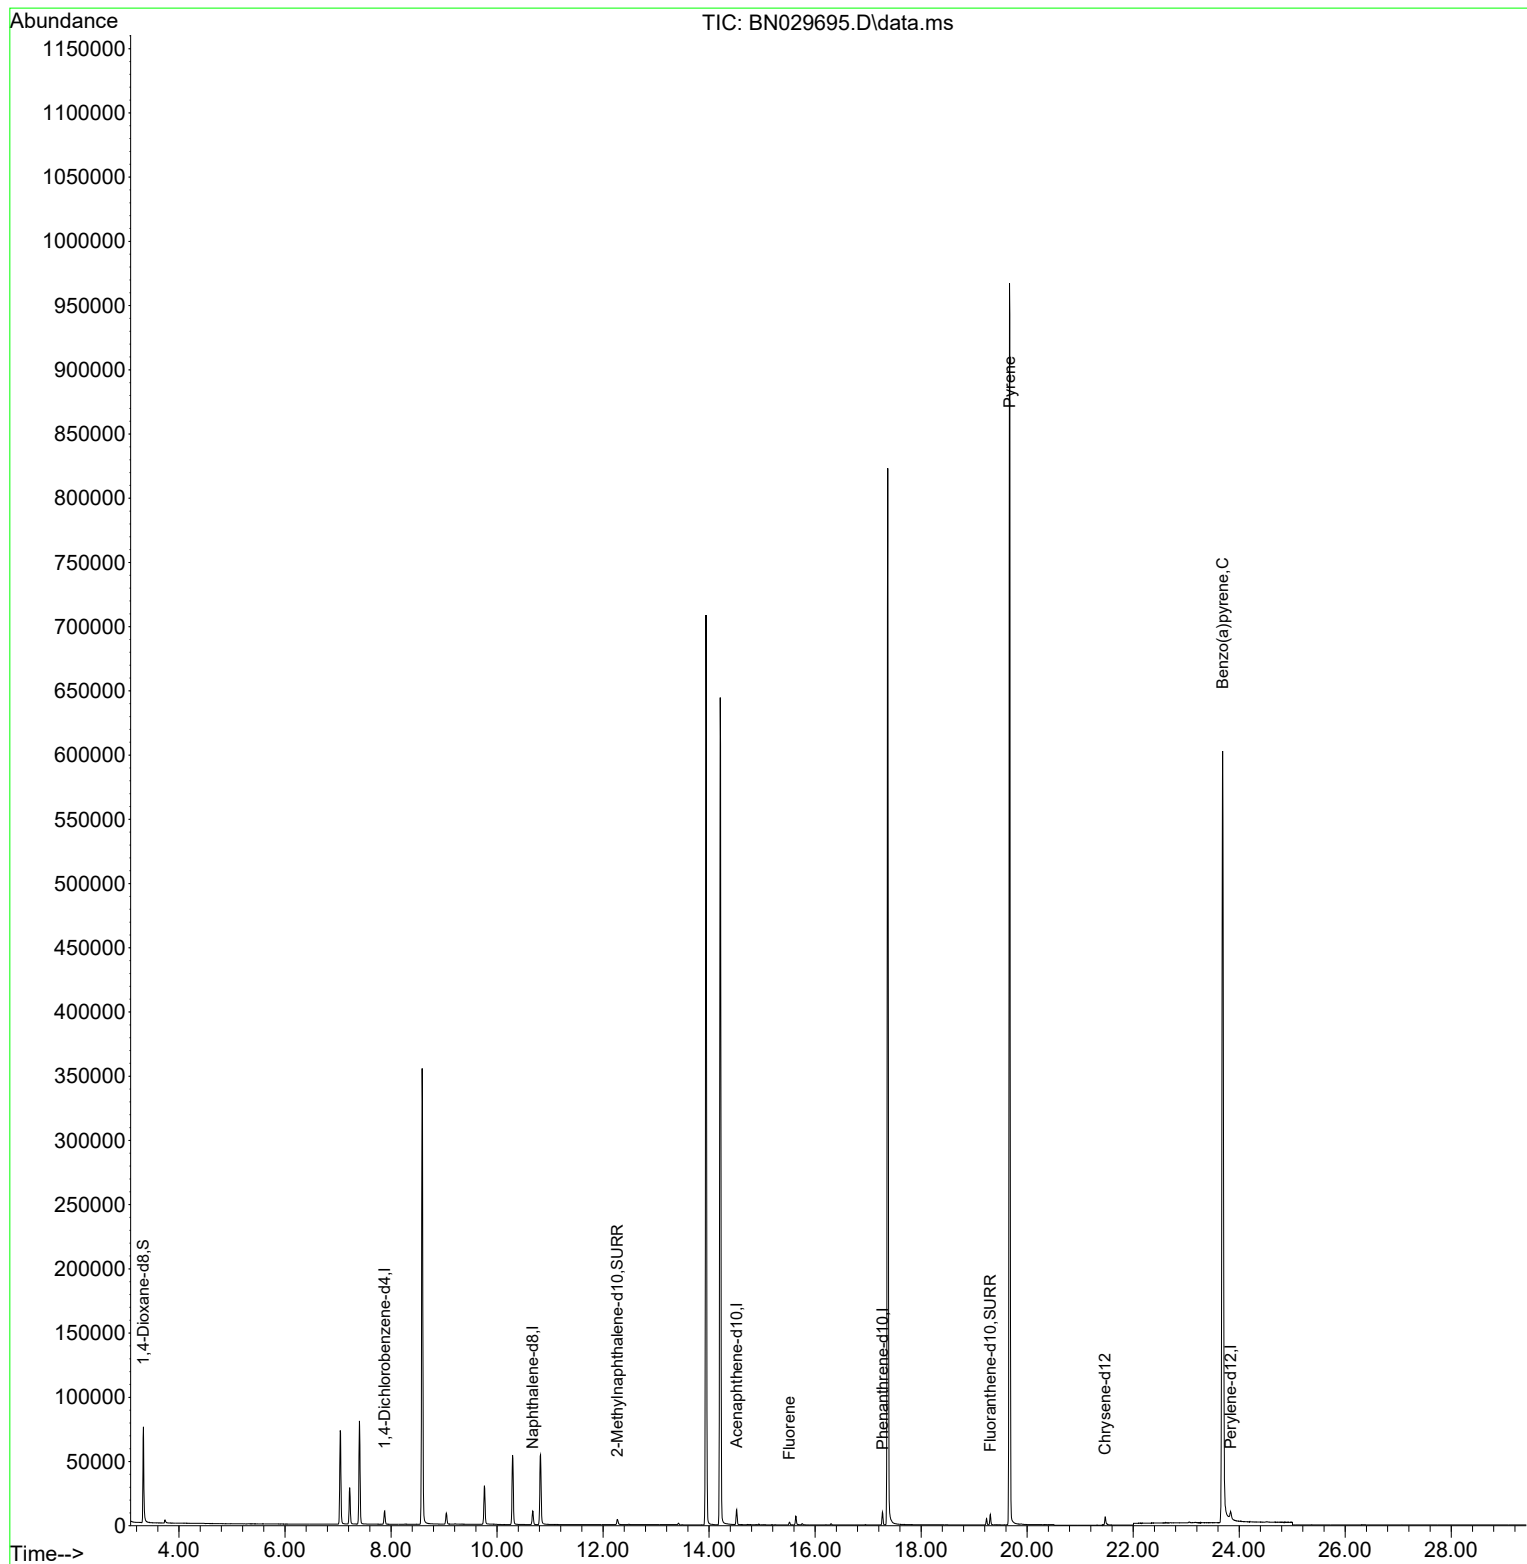


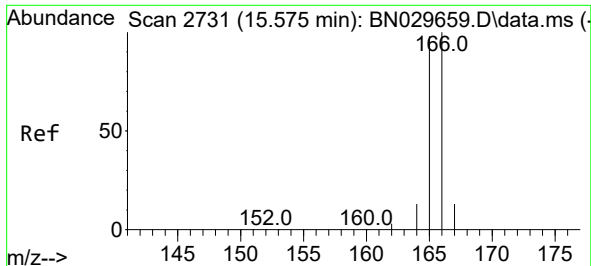

#12
 Fluorene
 Concen: 0.073 ng/ul
 RT: 15.515 min Scan# 21
 Delta R.T. -0.060 min
 Lab File: BN029695.D
 Acq: 11 Feb 2024 21:56




Instrument :
 BNA_N
 ClientSampleId :
 SBLK924


Tgt Ion:166 Resp: 1787
 Ion Ratio Lower Upper
 166 100
 165 10.4 78.6 117.8#
 167 34.5 11.5 17.3#

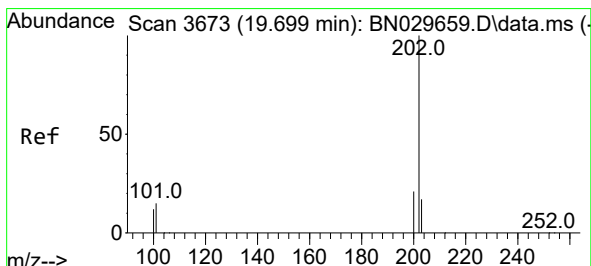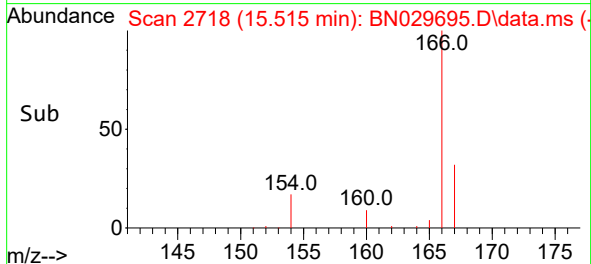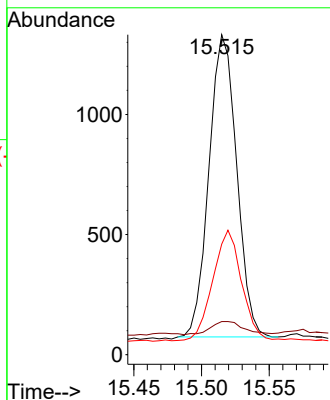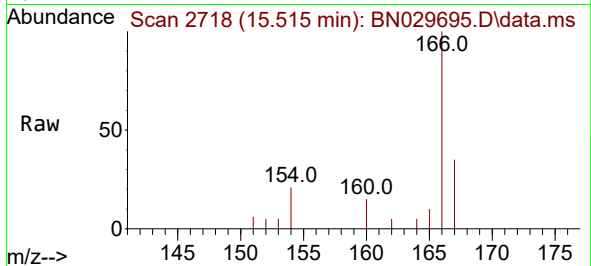

#20
 Pyrene
 Concen: 0.040 ng/ul
 RT: 19.671 min Scan# 3667
 Delta R.T. -0.028 min
 Lab File: BN029695.D
 Acq: 11 Feb 2024 21:56


Tgt Ion:202 Resp: 1438
 Ion Ratio Lower Upper
 202 100
 101 186.6 12.5 18.7#
 100 1355.3 10.0 15.0#

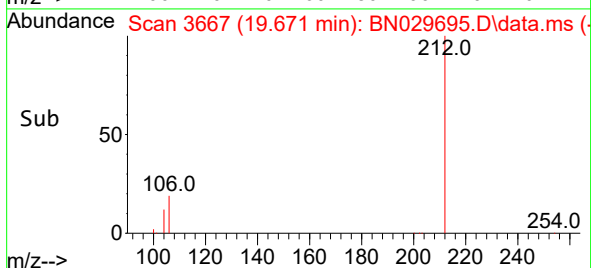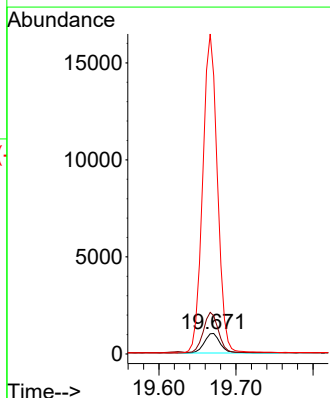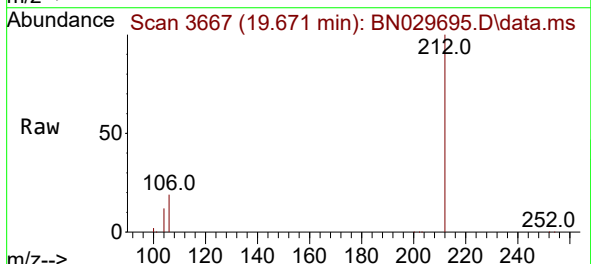

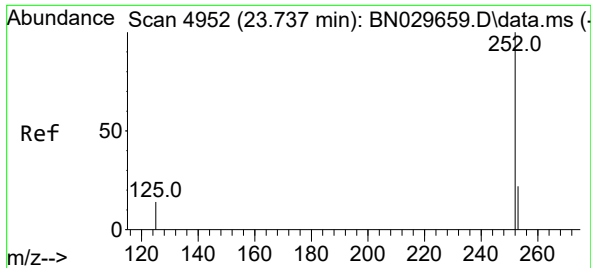

#26
Benzo(a)pyrene
Concen: 0.092 ng/ul
RT: 23.687 min Scan# 49
Delta R.T. -0.050 min
Lab File: BN029695.D
Acq: 11 Feb 2024 21:56

Instrument :
BNA_N
ClientSampleId :
SBLK924

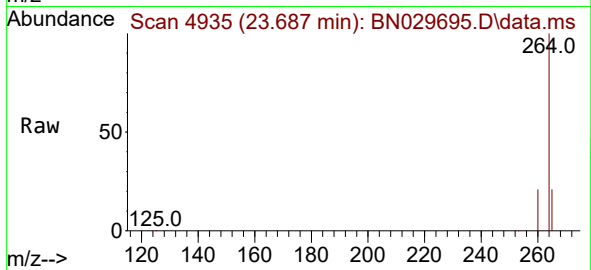

Tgt Ion:252 Resp: 3313
Ion Ratio Lower Upper
252 100
253 58.1 25.4 38.0#
125 39.2 16.0 24.0#

