

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN021124\  
 Data File : BN029666.D  
 Acq On : 11 Feb 2024 03:16  
 Operator : MA/JU  
 Sample : P1399-06  
 Misc :  
 ALS Vial : 58 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 C0AH9

Quant Time: Feb 11 23:24:30 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN020624.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sun Feb 11 23:18:17 2024  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| -----                       |        |      |          |       |        |          |
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.880  | 152  | 6020     | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.678 | 136  | 16650    | 0.400 | ng/ul  | 0.00     |
| 9) Acenaphthene-d10         | 14.520 | 164  | 7803     | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 17.272 | 188  | 15556    | 0.400 | ng/ul  | 0.00     |
| 17) Chrysene-d12            | 21.470 | 240  | 11445    | 0.400 | ng/ul  | 0.00     |
| 23) Perylene-d12            | 23.837 | 264  | 14919    | 0.400 | ng/ul  | 0.00     |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.332  | 96   | 35336    | 4.707 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.273 | 152  | 8623     | 0.407 | ng/ul  | 0.00     |
| 18) Fluoranthene-d10        | 19.304 | 212  | 16900    | 0.449 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       | Qvalue |          |
| 2) 1,4-Dioxane              | 3.370  | 88   | 1072     | 0.131 | ng/ul# | 78       |
| -----                       |        |      |          |       |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN021124\  
Data File : BN029666.D  
Acq On : 11 Feb 2024 03:16  
Operator : MA/JU  
Sample : P1399-06  
Misc :  
ALS Vial : 58 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
C0AH9

Quant Time: Feb 11 23:24:30 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN020624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sun Feb 11 23:18:17 2024  
Response via : Initial Calibration

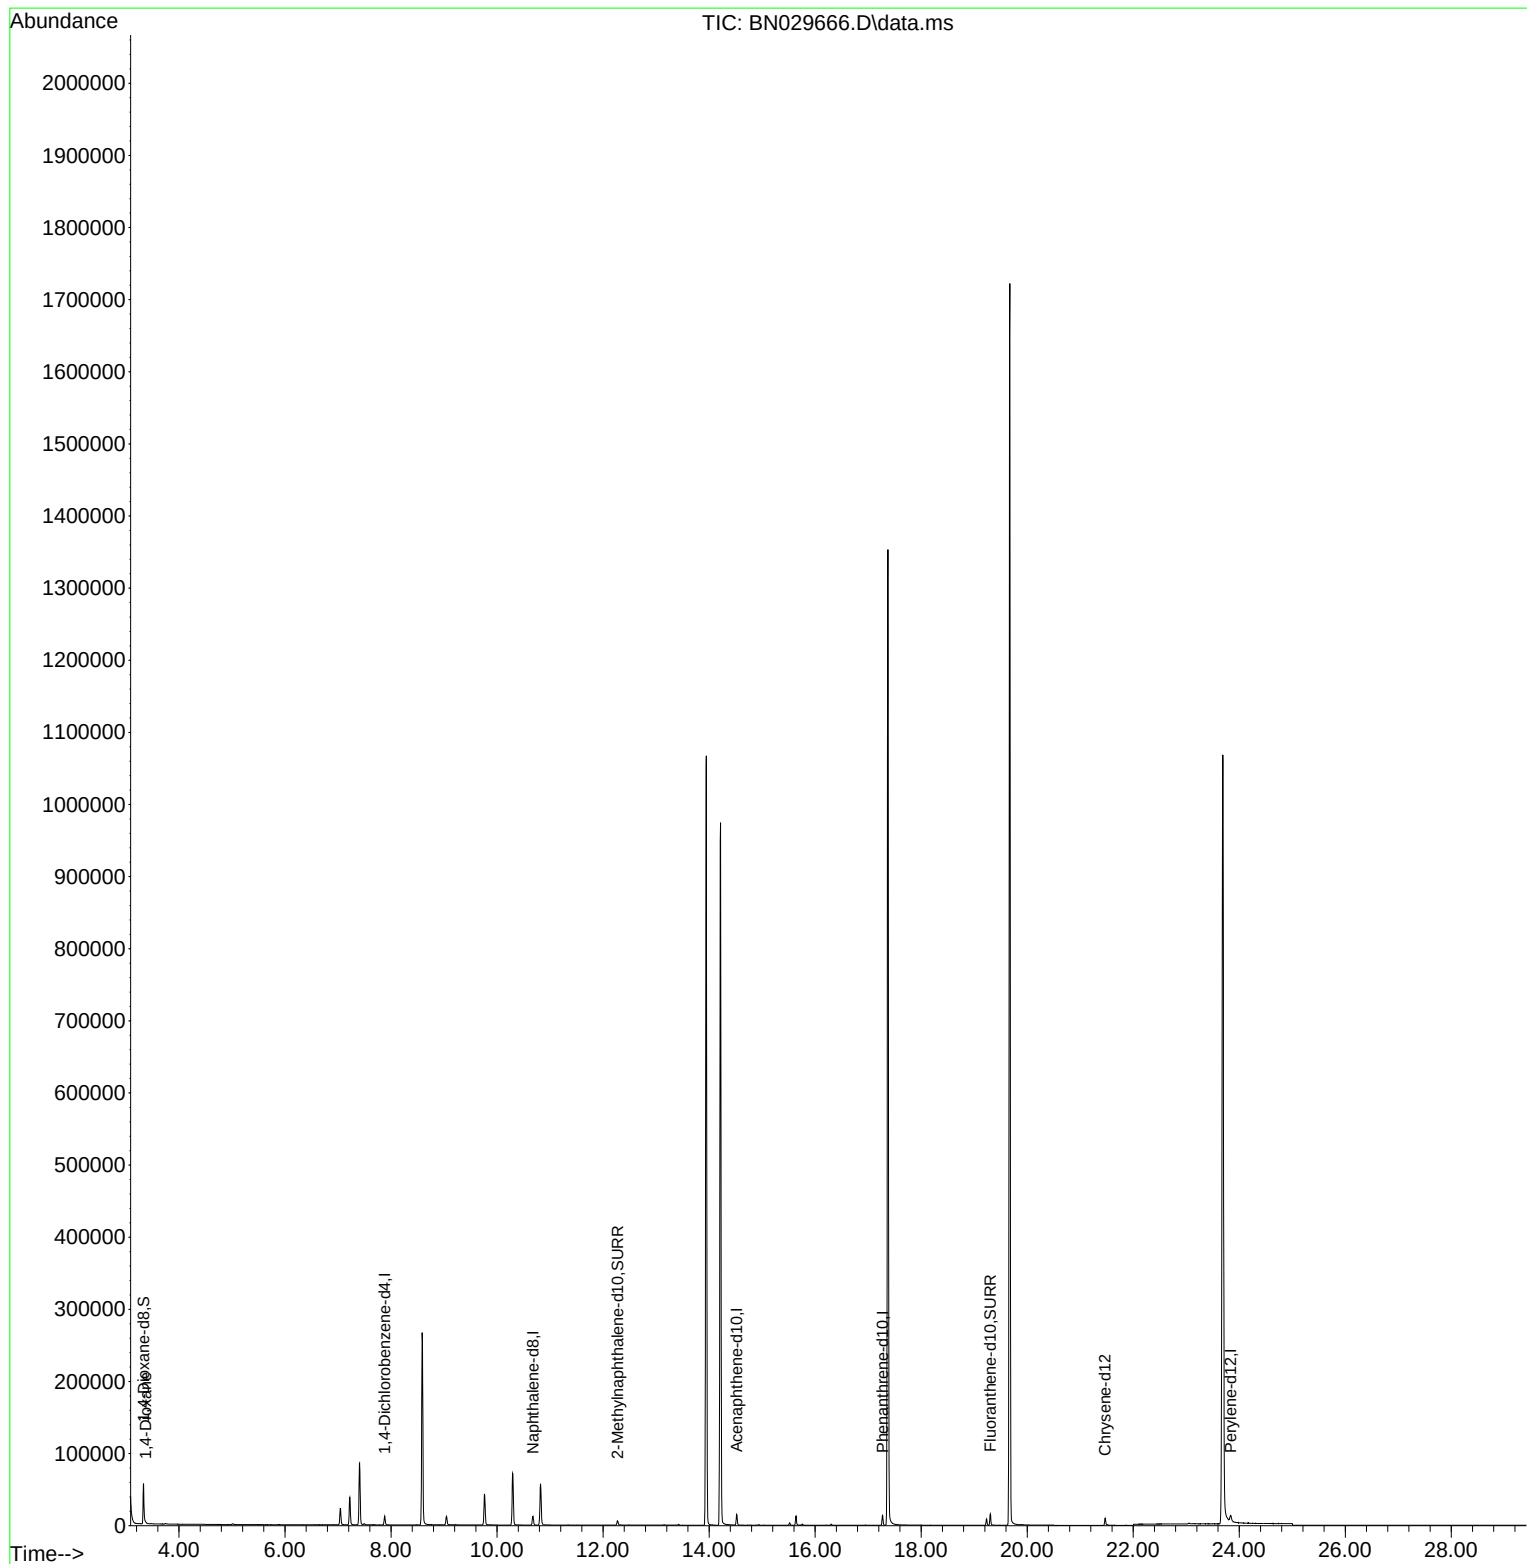

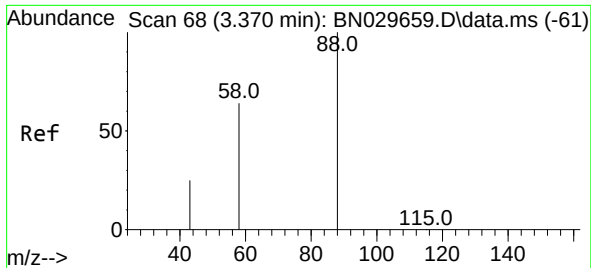

#2  
 1,4-Dioxane  
 Concen: 0.131 ng/ul  
 RT: 3.370 min Scan# 61  
 Delta R.T. 0.000 min  
 Lab File: BN029666.D  
 Acq: 11 Feb 2024 03:16

Instrument :  
 BNA\_N  
 ClientSampleId :  
 C0AH9

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 88    | Resp: | 1072  |
| Ion      | Ratio | Lower | Upper |
| 88       | 100   |       |       |
| 43       | 27.3  | 21.8  | 32.6  |
| 58       | 26.2  | 39.3  | 58.9  |

