

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029667.D
 Acq On : 11 Feb 2024 03:52
 Operator : MA/JU
 Sample : P1399-07
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ0

Quant Time: Feb 11 23:24:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	6255	0.400	ng/u1	0.00
4) Naphthalene-d8	10.678	136	17212	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.520	164	7733	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.272	188	14298	0.400	ng/u1	0.00
17) Chrysene-d12	21.470	240	10331	0.400	ng/u1	0.00
23) Perylene-d12	23.837	264	13298	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	34273	4.394	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.273	152	8978	0.410	ng/u1	0.00
18) Fluoranthene-d10	19.304	212	14493	0.427	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.366	88	1591	0.187	ng/u1	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\  
Data File : BN029667.D  
Acq On    : 11 Feb 2024   03:52  
Operator  : MA/JU  
Sample    : P1399-07  
Misc      :  
ALS Vial  : 59    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
C0AJ0

Quant Time: Feb 11 23:24:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration

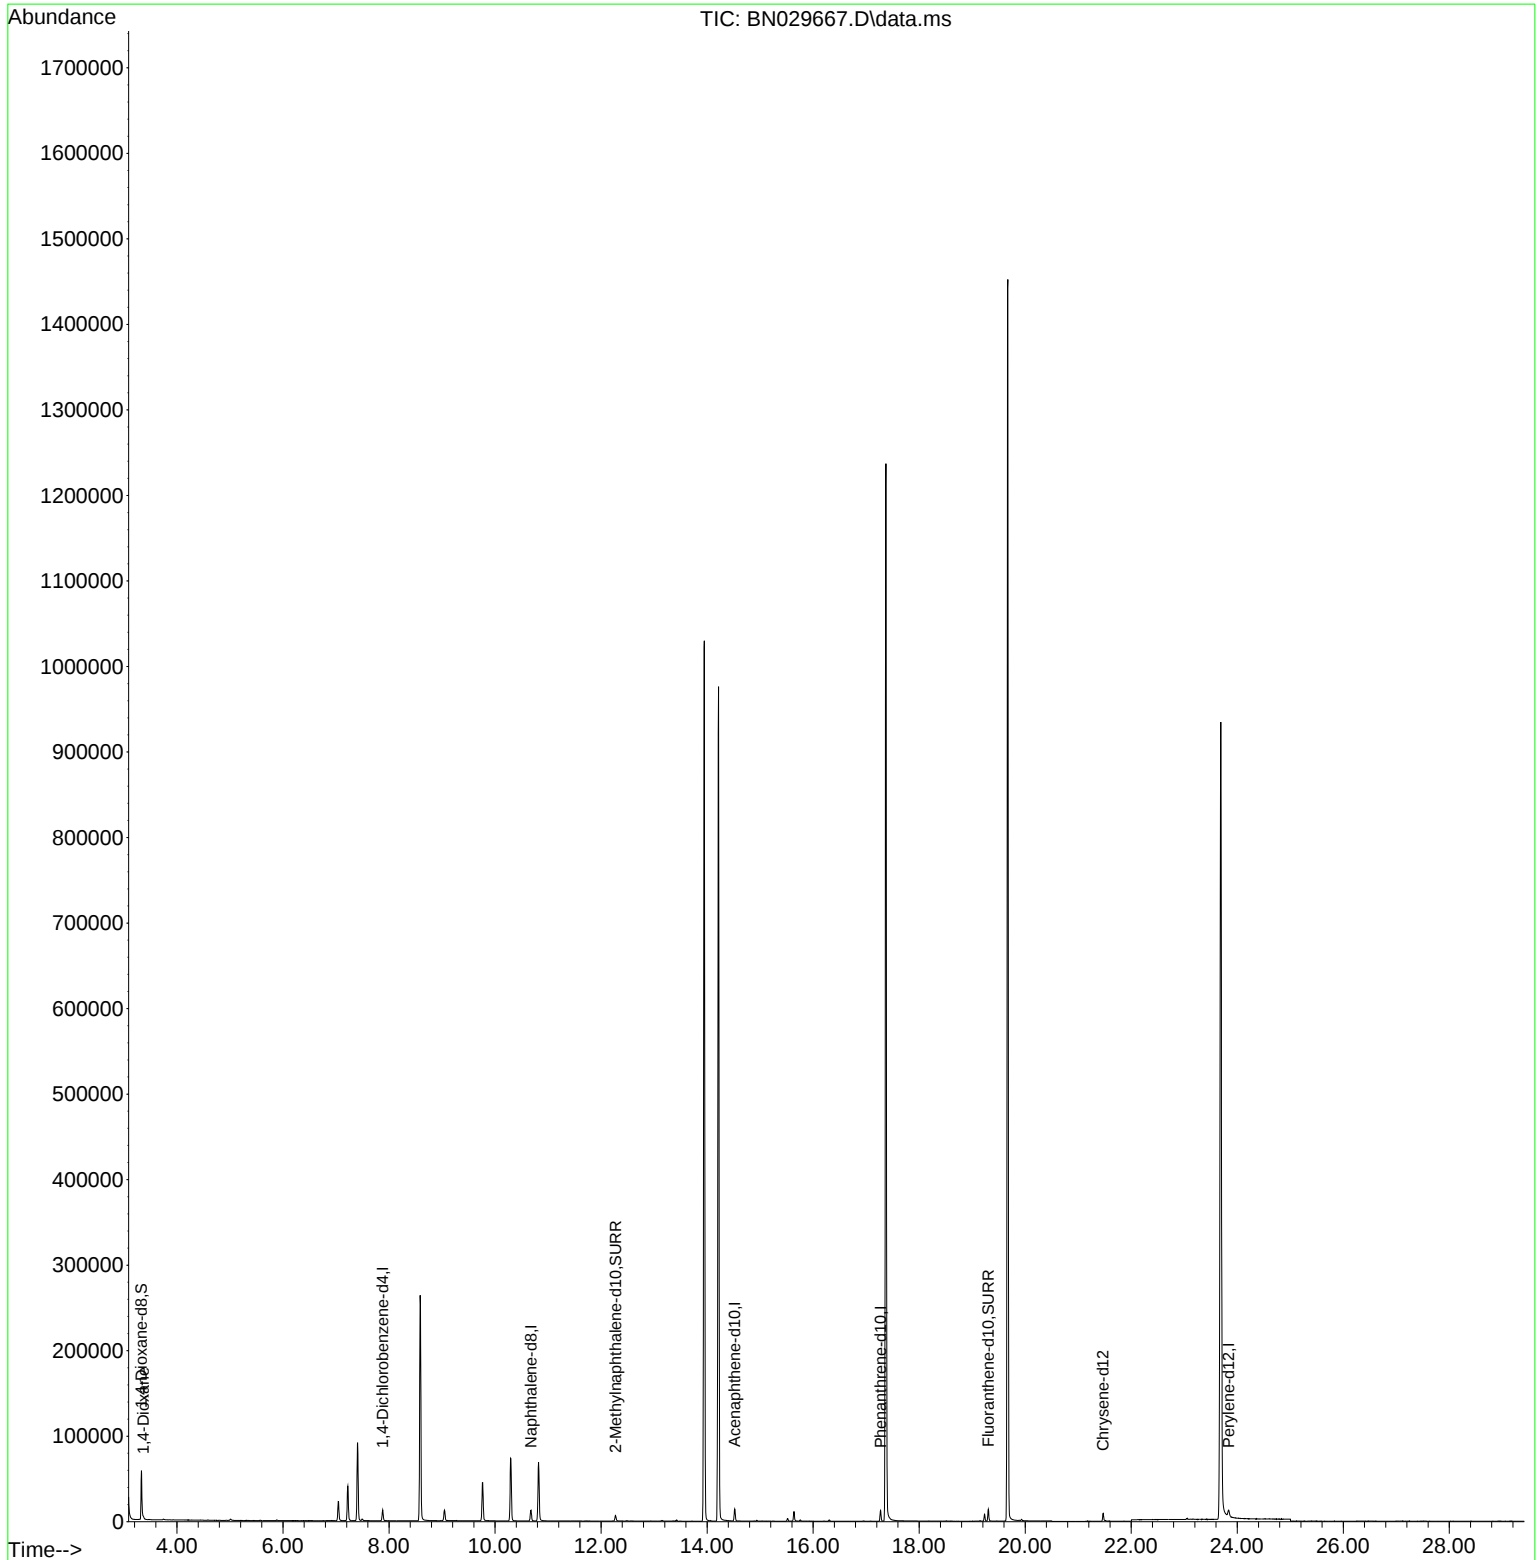

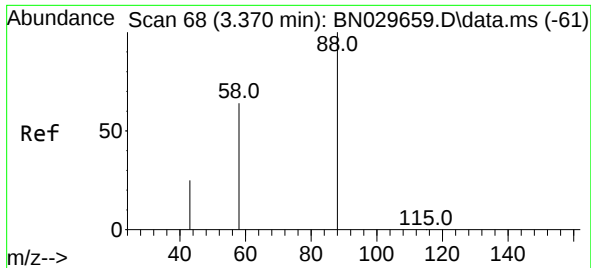

#2
 1,4-Dioxane
 Concen: 0.187 ng/ul
 RT: 3.366 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN029667.D
 Acq: 11 Feb 2024 03:52

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ0

Tgt Ion: 88 Resp: 1591

Ion	Ratio	Lower	Upper
88	100		
43	32.2	21.8	32.6
58	39.4	39.3	58.9

