

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029670.D
 Acq On : 11 Feb 2024 05:41
 Operator : MA/JU
 Sample : P1399-10
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ3

Quant Time: Feb 11 23:24:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	5759	0.400	ng/ul	0.00
4) Naphthalene-d8	10.678	136	15739	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.520	164	7158	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.272	188	13643	0.400	ng/ul	0.00
17) Chrysene-d12	21.473	240	9668	0.400	ng/ul	0.00
23) Perylene-d12	23.840	264	13029	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	37602	5.236	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.272	152	9070	0.453	ng/ul	0.00
18) Fluoranthene-d10	19.304	212	14724	0.463	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.370	88	525	0.067	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
Data File : BN029670.D
Acq On : 11 Feb 2024 05:41
Operator : MA/JU
Sample : P1399-10
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ3

Quant Time: Feb 11 23:24:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration

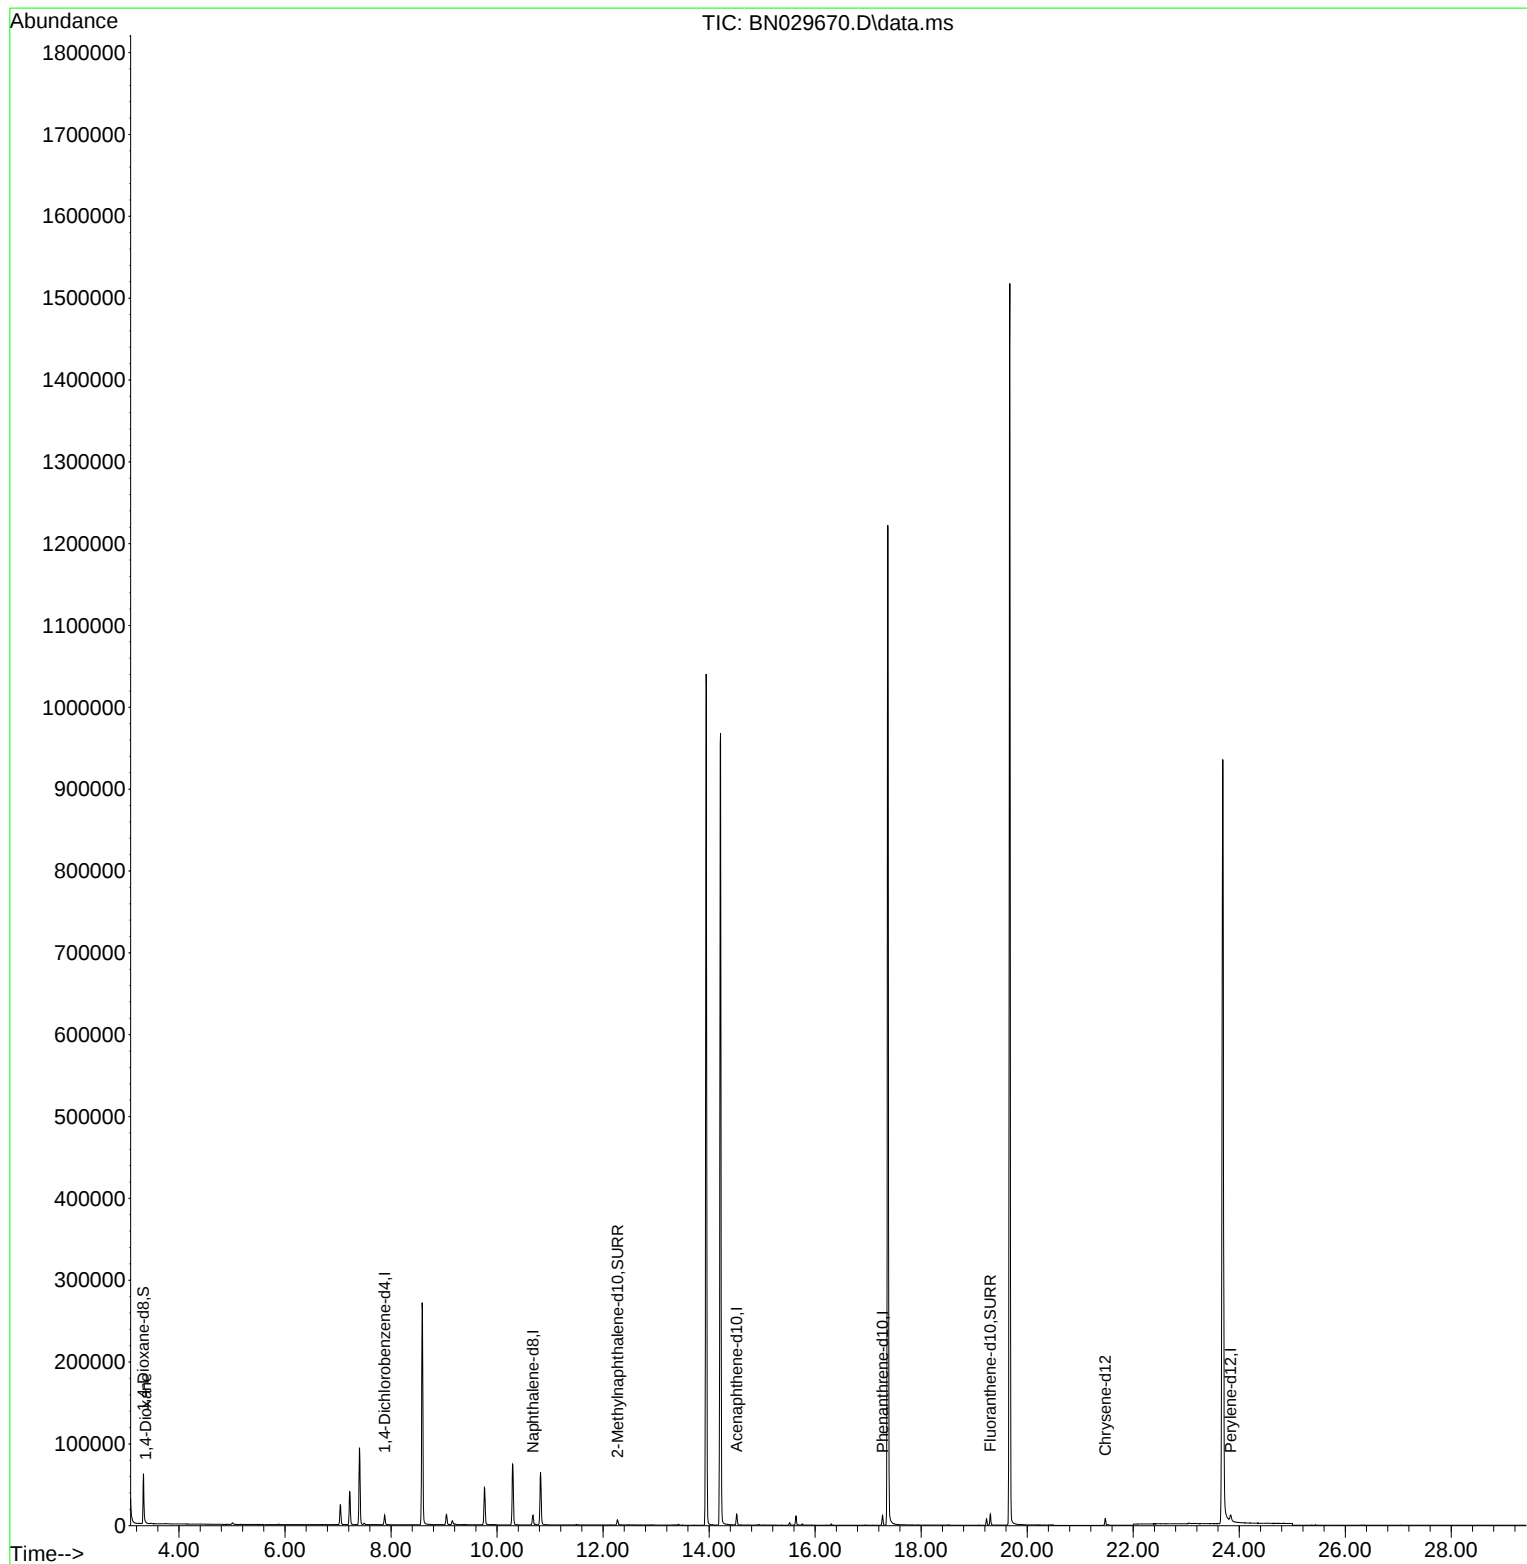

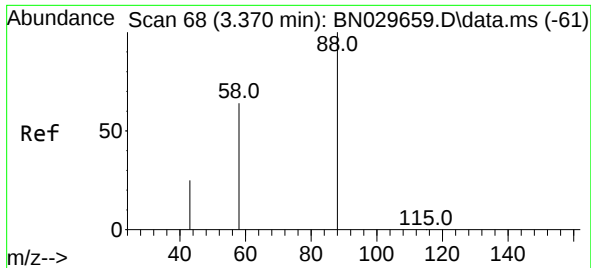

#2
 1,4-Dioxane
 Concen: 0.067 ng/ul
 RT: 3.370 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN029670.D
 Acq: 11 Feb 2024 05:41

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ3

Tgt Ion:	88	Resp:	525
Ion	Ratio	Lower	Upper
88	100		
43	29.5	21.8	32.6
58	16.5	39.3	58.9#

