

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029671.D
 Acq On : 11 Feb 2024 06:16
 Operator : MA/JU
 Sample : P1399-11
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ4

Quant Time: Feb 11 23:25:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	5740	0.400	ng/ul	0.00
4) Naphthalene-d8	10.676	136	15973	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.519	164	7157	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.271	188	12985	0.400	ng/ul	0.00
17) Chrysene-d12	21.473	240	8899	0.400	ng/ul	0.00
23) Perylene-d12	23.837	264	12220	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.332	96	35019	4.893	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.271	152	7746	0.381	ng/ul	0.00
18) Fluoranthene-d10	19.307	212	13571	0.464	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.370	88	546	0.070	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
Data File : BN029671.D
Acq On : 11 Feb 2024 06:16
Operator : MA/JU
Sample : P1399-11
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ4

Quant Time: Feb 11 23:25:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration

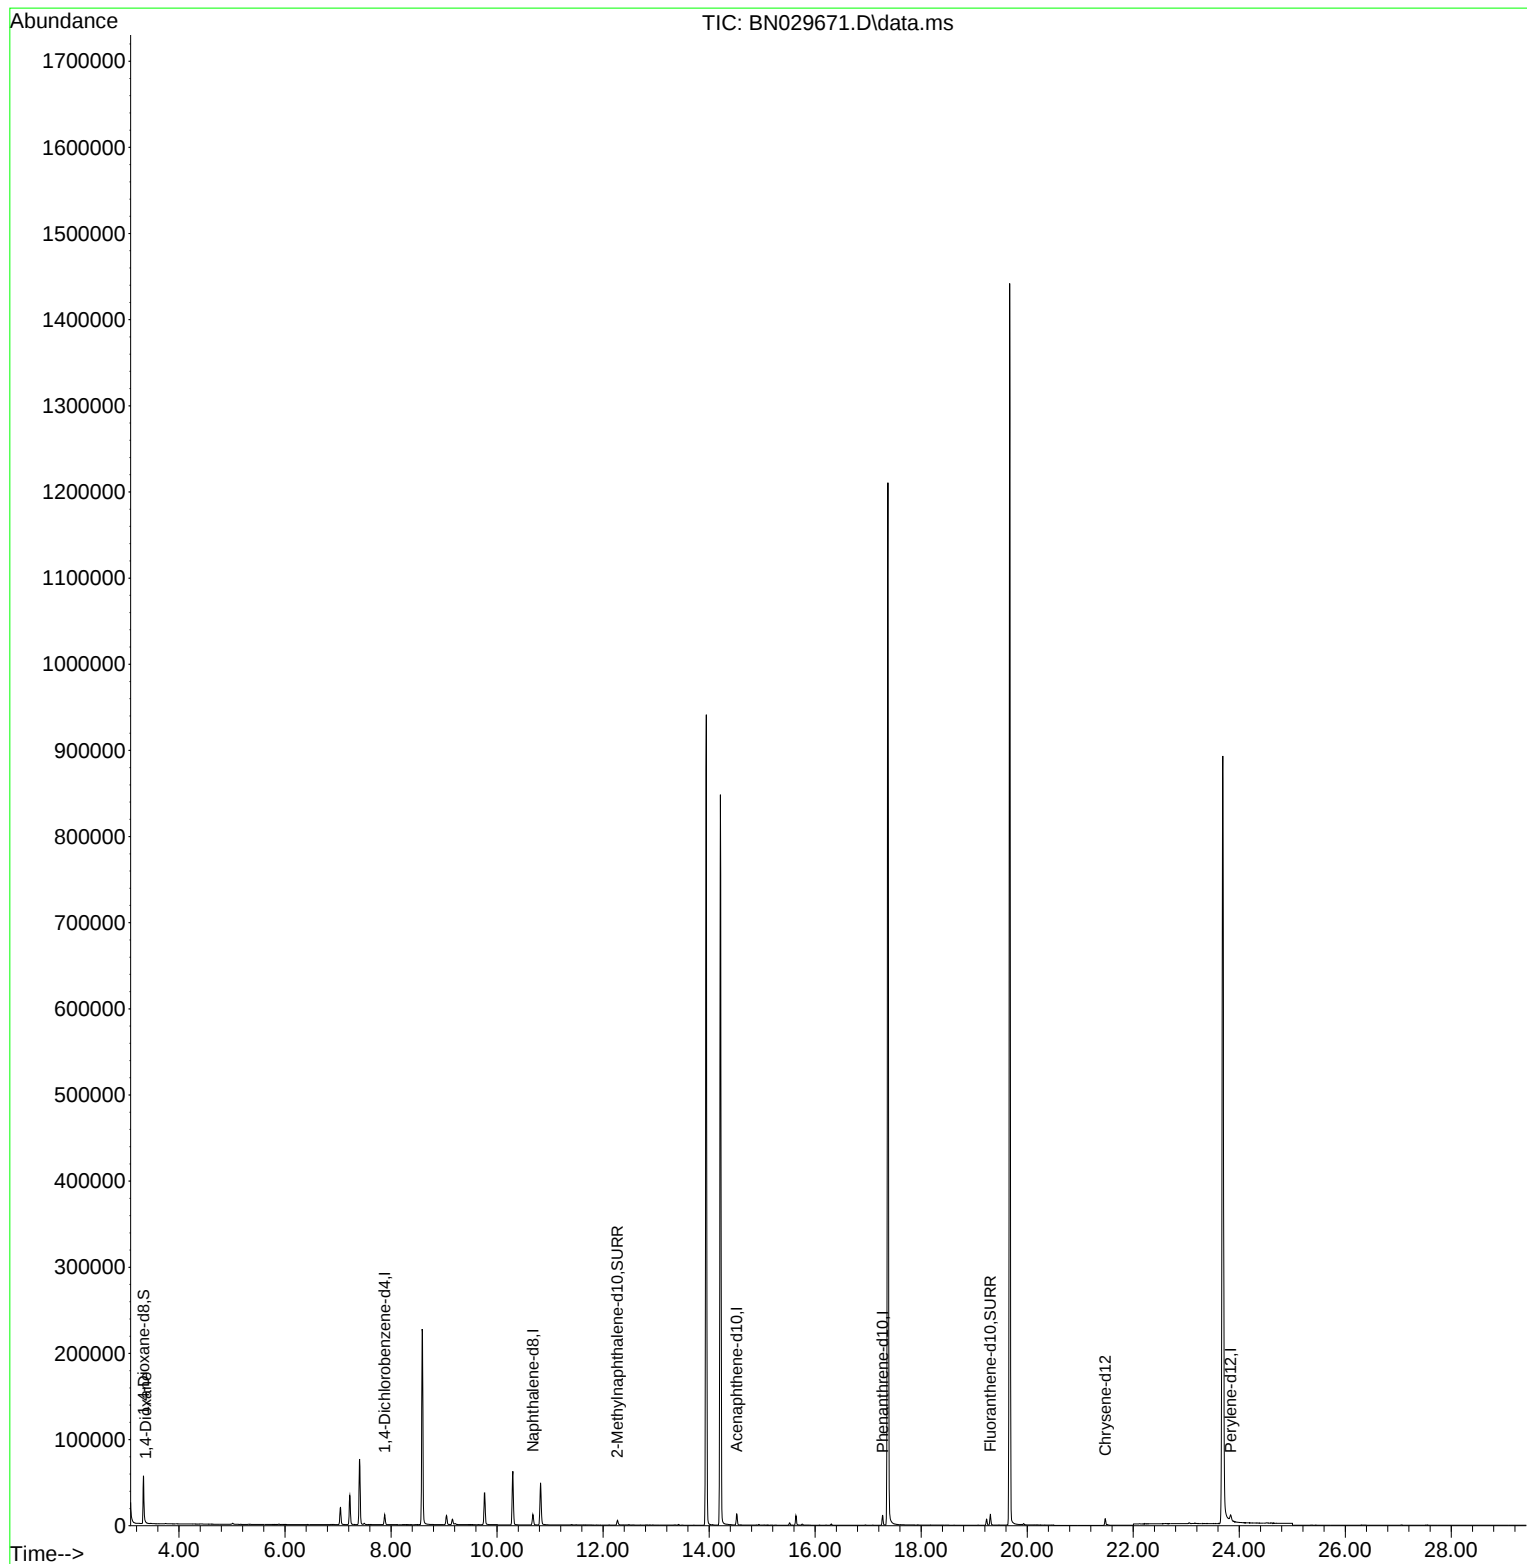

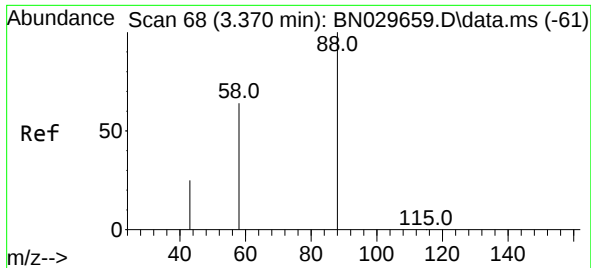

#2
 1,4-Dioxane
 Concen: 0.070 ng/ul
 RT: 3.370 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN029671.D
 Acq: 11 Feb 2024 06:16

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ4

Tgt Ion:	88	Resp:	546
Ion	Ratio	Lower	Upper
88	100		
43	29.7	21.8	32.6
58	18.4	39.3	58.9

