

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029686.D
 Acq On : 11 Feb 2024 15:55
 Operator : MA/JU
 Sample : P1399-01
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH4

Quant Time: Feb 11 23:27:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	6492	0.400	ng/ul	0.00
4) Naphthalene-d8	10.672	136	18229	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.520	164	8663	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.272	188	15145	0.400	ng/ul	0.00
17) Chrysene-d12	21.473	240	9897	0.400	ng/ul	0.00
23) Perylene-d12	23.840	264	12912	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	38602	4.769	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.267	152	9757	0.421	ng/ul	0.00
18) Fluoranthene-d10	19.304	212	15374	0.473	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.366	88	2849	0.323	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
Data File : BN029686.D
Acq On : 11 Feb 2024 15:55
Operator : MA/JU
Sample : P1399-01
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH4

Quant Time: Feb 11 23:27:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration

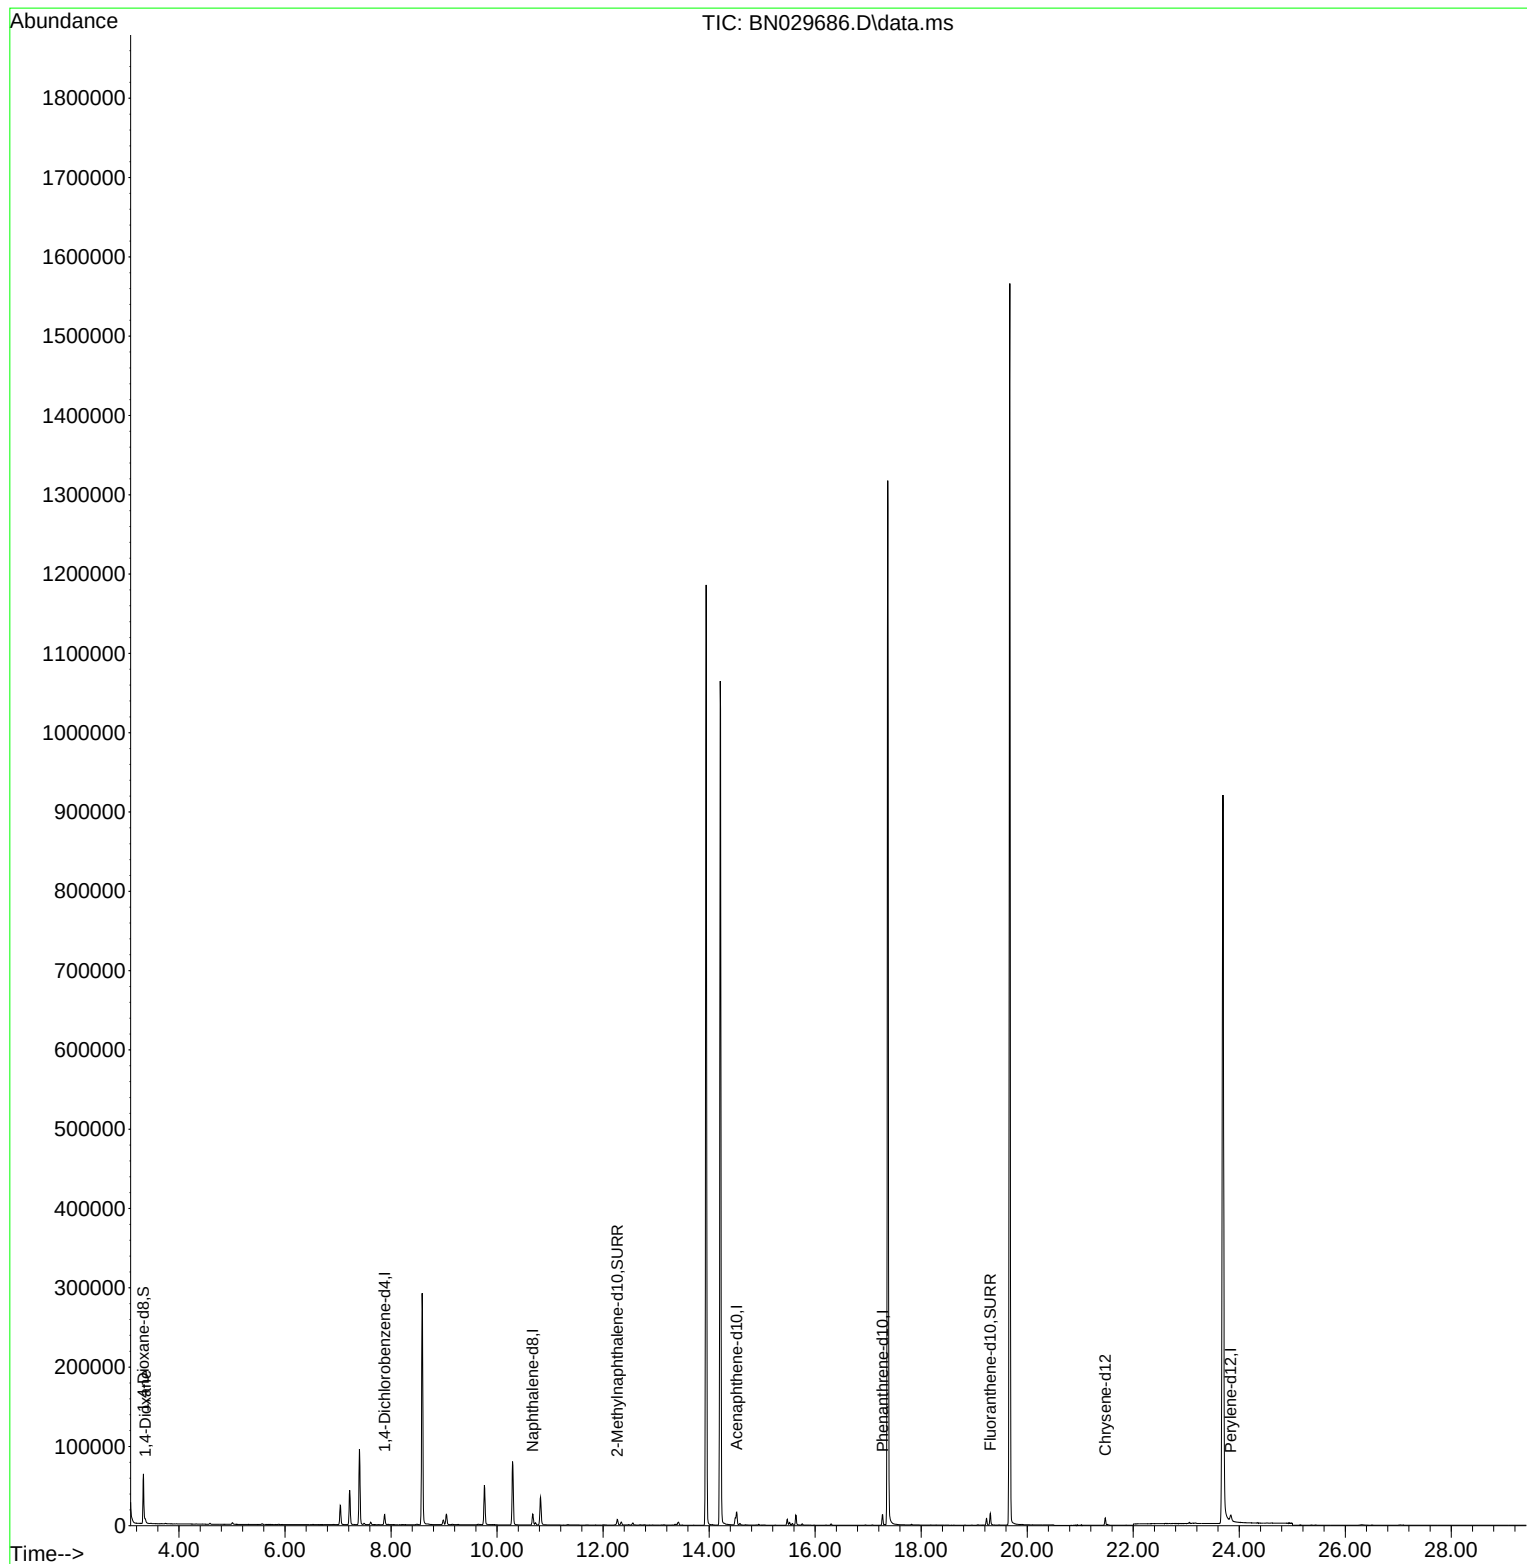

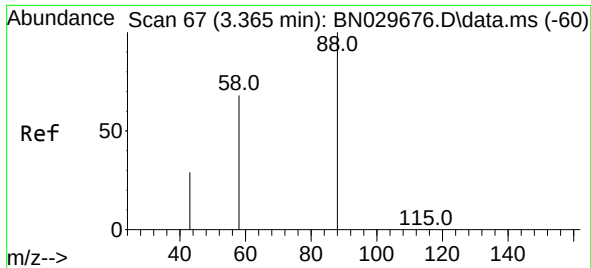

#2
 1,4-Dioxane
 Concen: 0.323 ng/ul
 RT: 3.366 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN029686.D
 Acq: 11 Feb 2024 15:55

Instrument :
 BNA_N
 ClientSampleId :
 C0AH4

Tgt Ion:	88	Resp:	2849
Ion	Ratio	Lower	Upper
88	100		
43	34.1	21.8	32.6#
58	47.1	39.3	58.9

