

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
 Data File : BN029701.D
 Acq On : 12 Feb 2024 01:34
 Operator : MA/JU
 Sample : P1398-15
 Misc :
 ALS Vial : 95 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG8

Quant Time: Feb 12 02:02:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Feb 11 23:18:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.876	152	4902	0.400	ng/ul	0.00
4) Naphthalene-d8	10.672	136	13308	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.520	164	5995	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.272	188	11147	0.400	ng/ul	0.00
17) Chrysene-d12	21.469	240	7865	0.400	ng/ul	0.00
23) Perylene-d12	23.836	264	10511	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	27790	4.547	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.267	152	6500	0.384	ng/ul	0.00
18) Fluoranthene-d10	19.304	212	12839	0.497	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.370	88	1170	0.176	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021124\
Data File : BN029701.D
Acq On : 12 Feb 2024 01:34
Operator : MA/JU
Sample : P1398-15
Misc :
ALS Vial : 95 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG8


Quant Time: Feb 12 02:02:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Feb 11 23:18:17 2024
Response via : Initial Calibration

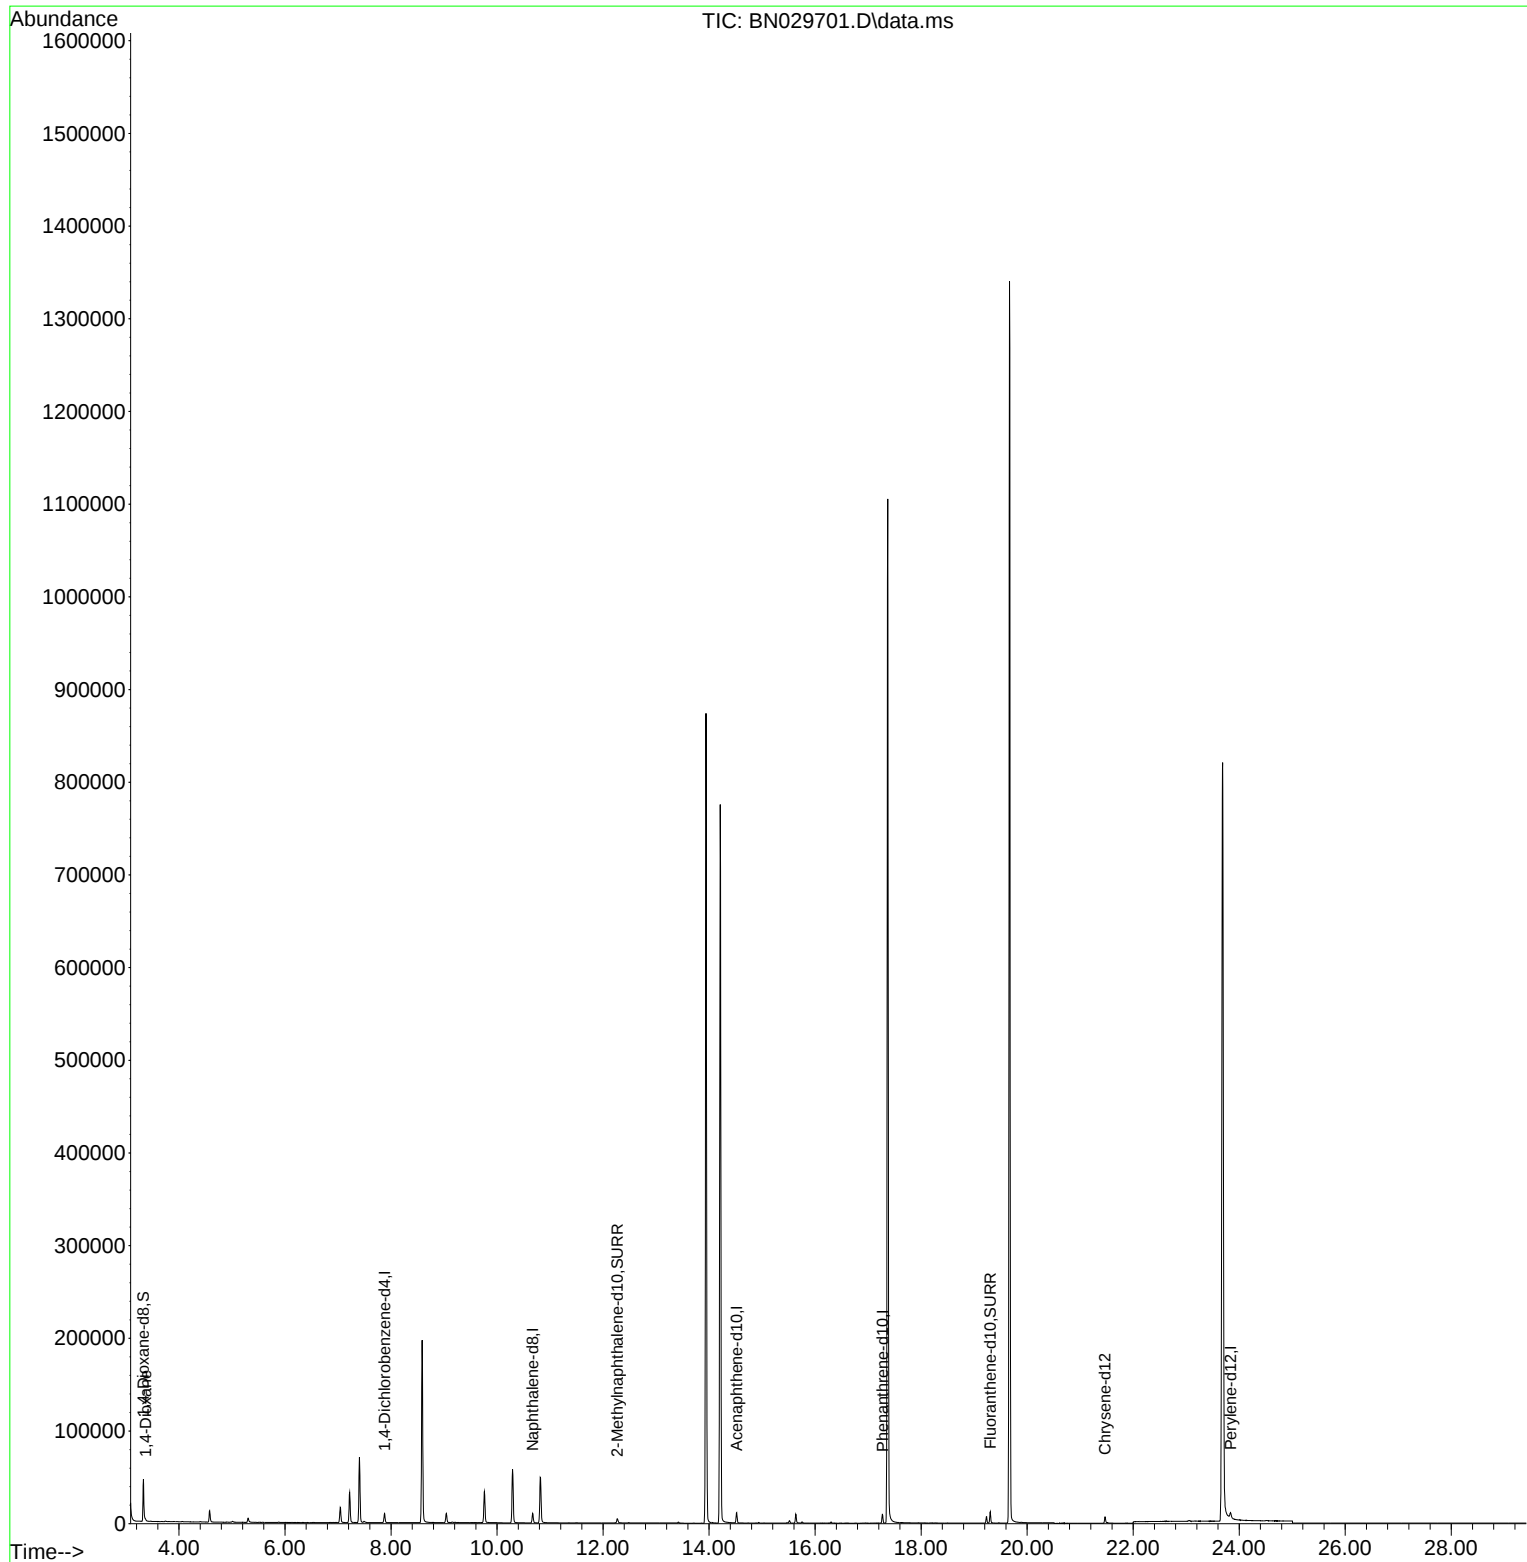

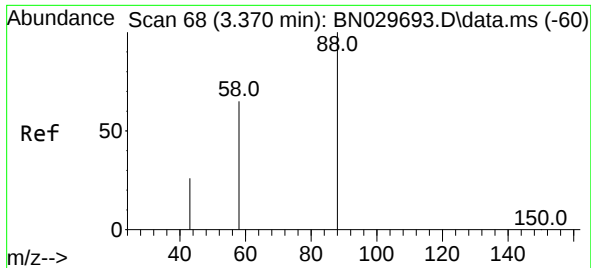

#2
 1,4-Dioxane
 Concen: 0.176 ng/ul
 RT: 3.370 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN029701.D
 Acq: 12 Feb 2024 01:34

Instrument :
 BNA_N
 ClientSampleId :
 C0AG8

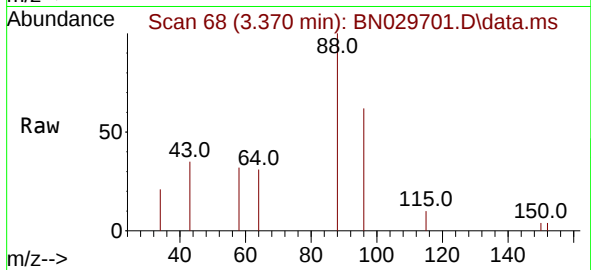

Tgt Ion: 88 Resp: 1170
 Ion Ratio Lower Upper
 88 100
 43 34.8 21.8 32.6#
 58 31.5 39.3 58.9#

