
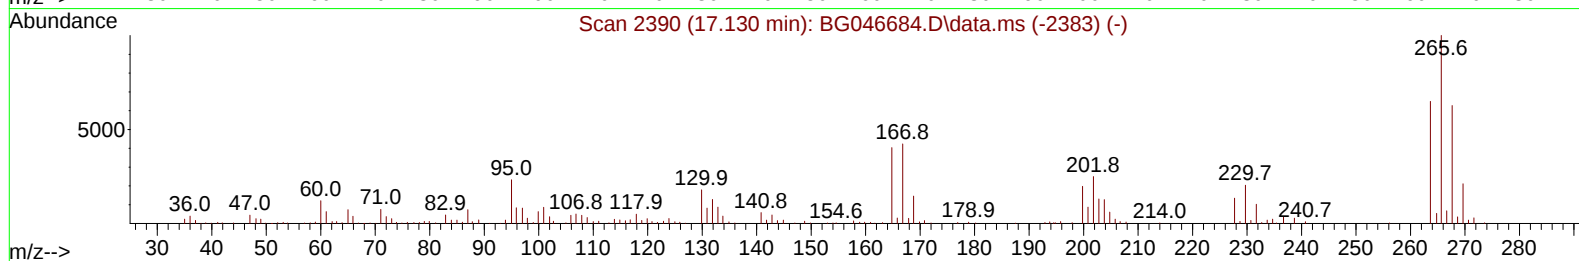
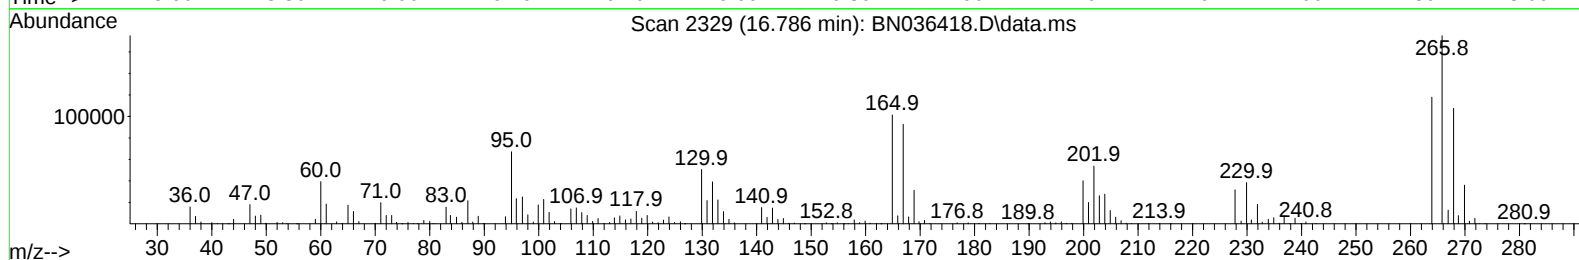


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021125\
Data File : BN036418.D
Acq On : 11 Feb 2025 09:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 17:47:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

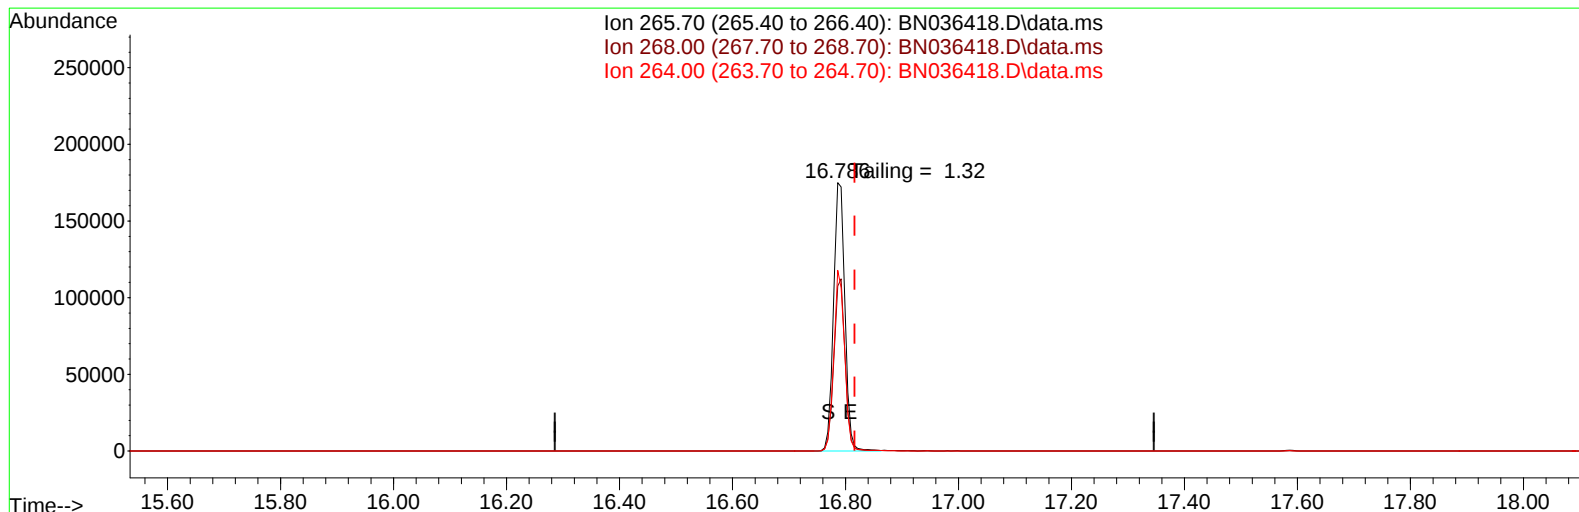

TIC: BN036418.D\data.ms

(70) Pentachlorophenol (C)




16.786min (-0.029) 20524.85 ng

response 244188

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.46
264.00	61.60	67.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021125\
Data File : BN036418.D
Acq On : 11 Feb 2025 09:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 17:47:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

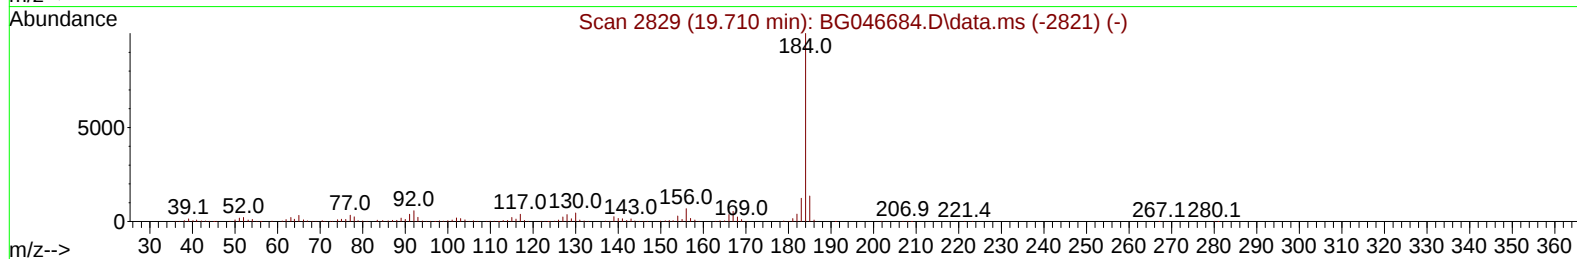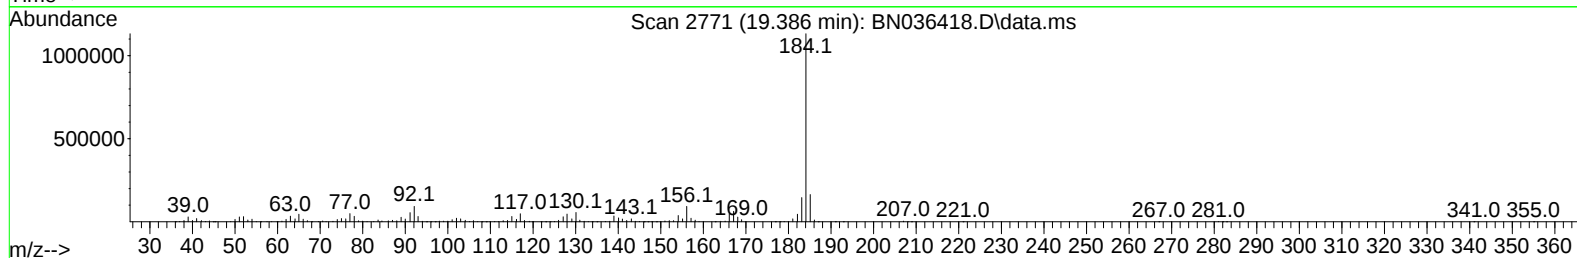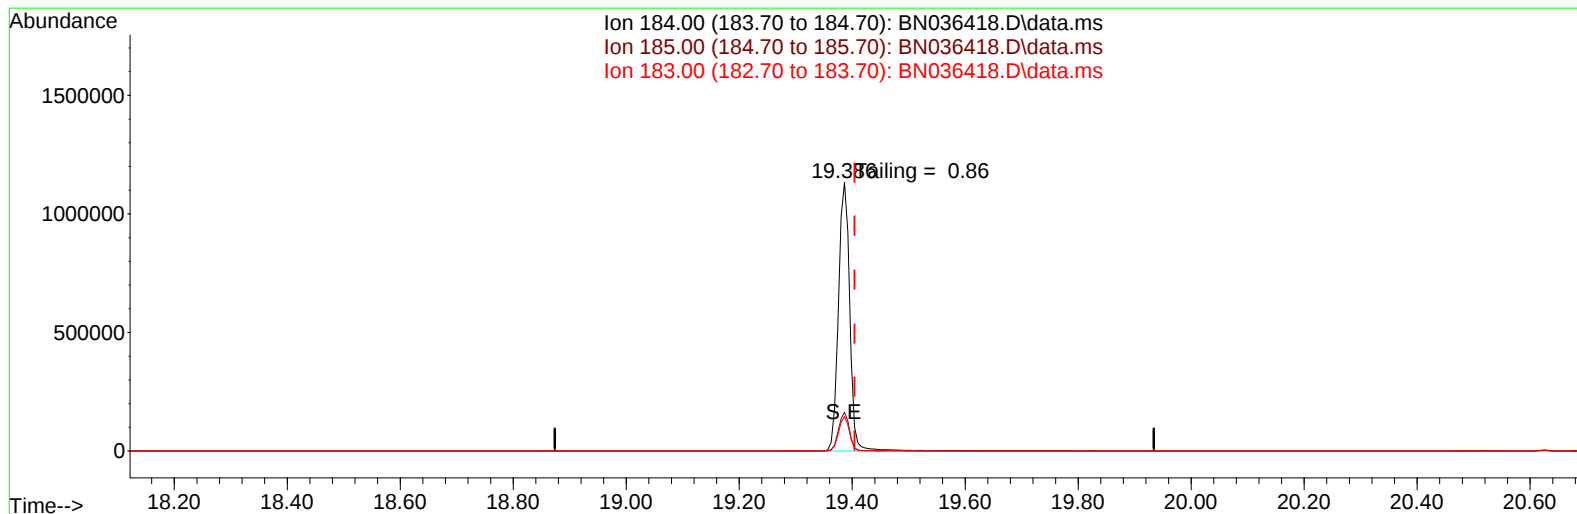

TIC: BN036418.D\data.ms

(77) Benzdine

19.386min (-0.018) 0.00 ng

response 1568249

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.52
183.00	13.20	12.85
0.00	0.00	0.00