


Data Path : Z:\HPCHEM1\BNA N\Data\BN021218\
 Data File : BN000058.D
 Acq On : 12 Feb 2018 09:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 18:24:45 2018

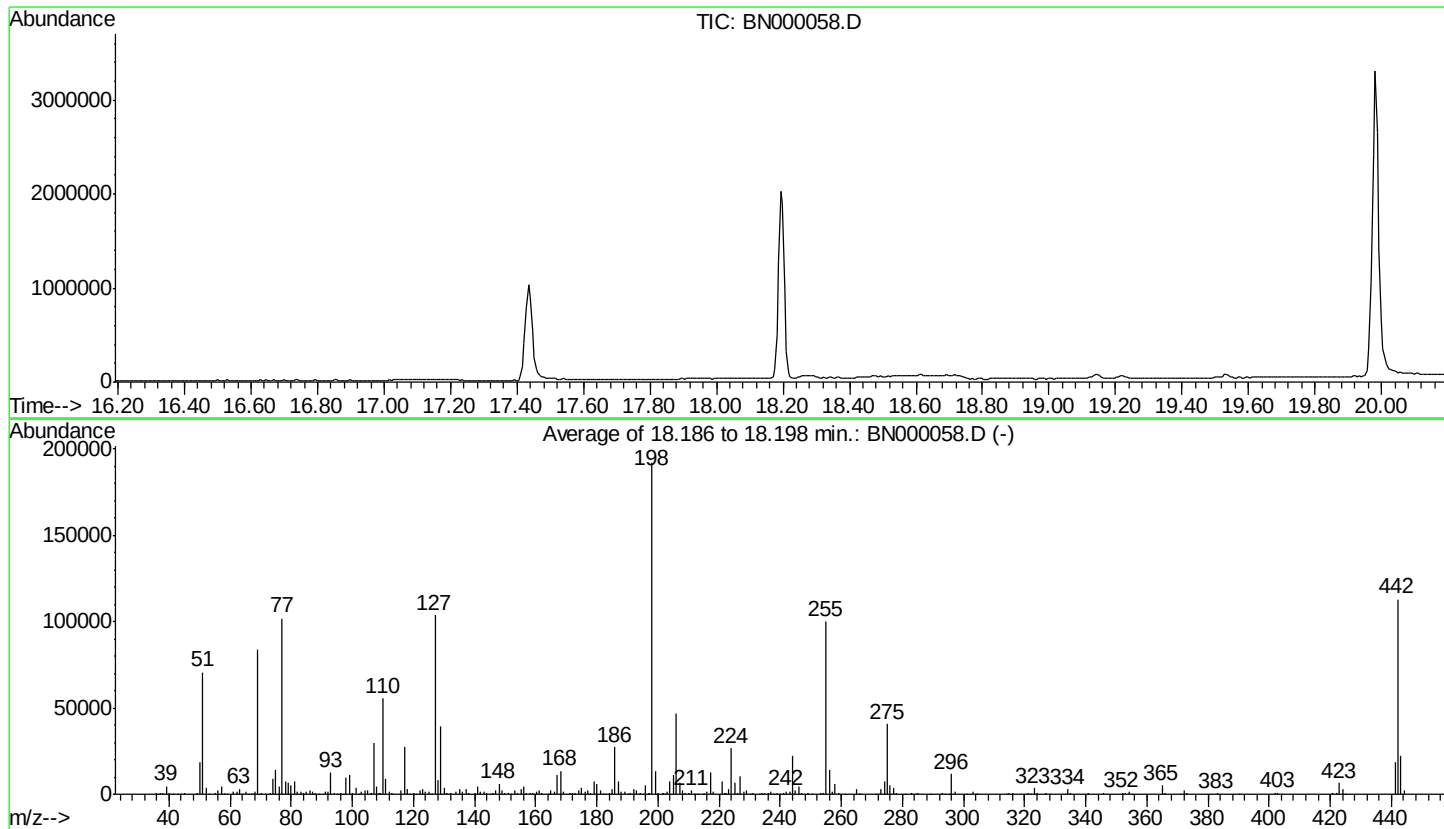

AutoFind: Scans 2584, 2585, 2586; Background Corrected with Scan 2578

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	70830	PASS
68	69	0.00	2	1.9	1615	PASS
69	198	0.00	100	43.7	84070	PASS
70	69	0.00	2	0.8	701	PASS
127	198	10	80	53.9	103645	PASS
197	198	0.00	2	0.6	1069	PASS
198	198	100	100	100.0	192192	PASS
199	198	5	9	6.9	13283	PASS
275	198	10	60	21.1	40557	PASS
365	198	1	100	2.6	4975	PASS
441	443	0.01	100	83.3	18465	PASS
442	198	50	100	58.7	112818	PASS
443	442	15	24	19.6	22157	PASS