
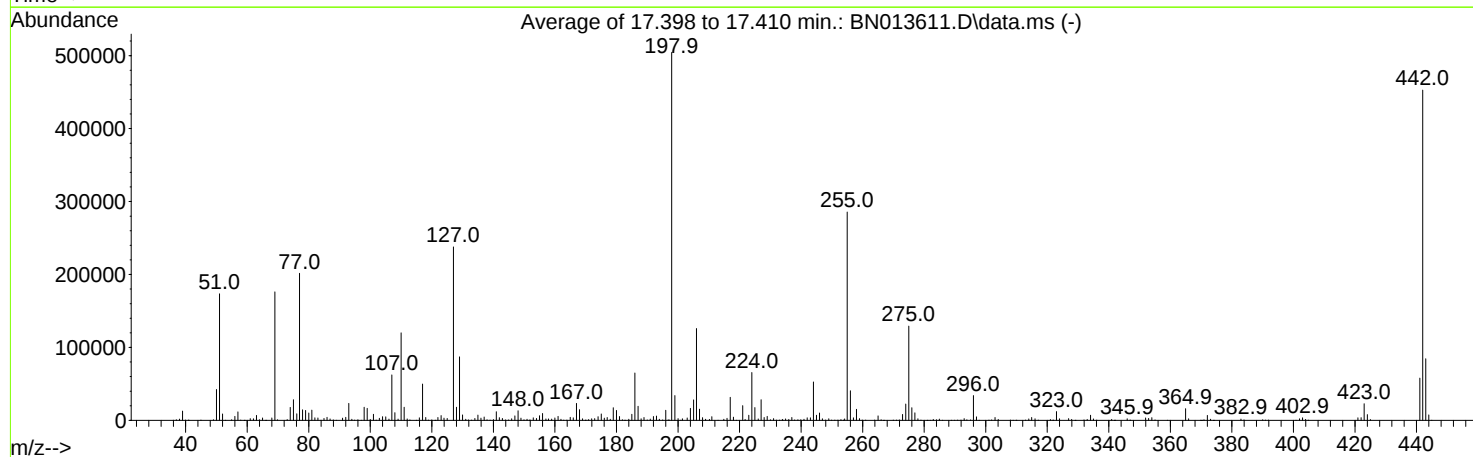


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021221\
 Data File : BN013611.D
 Acq On : 12 Feb 2021 13:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 08 15:13:18 2021

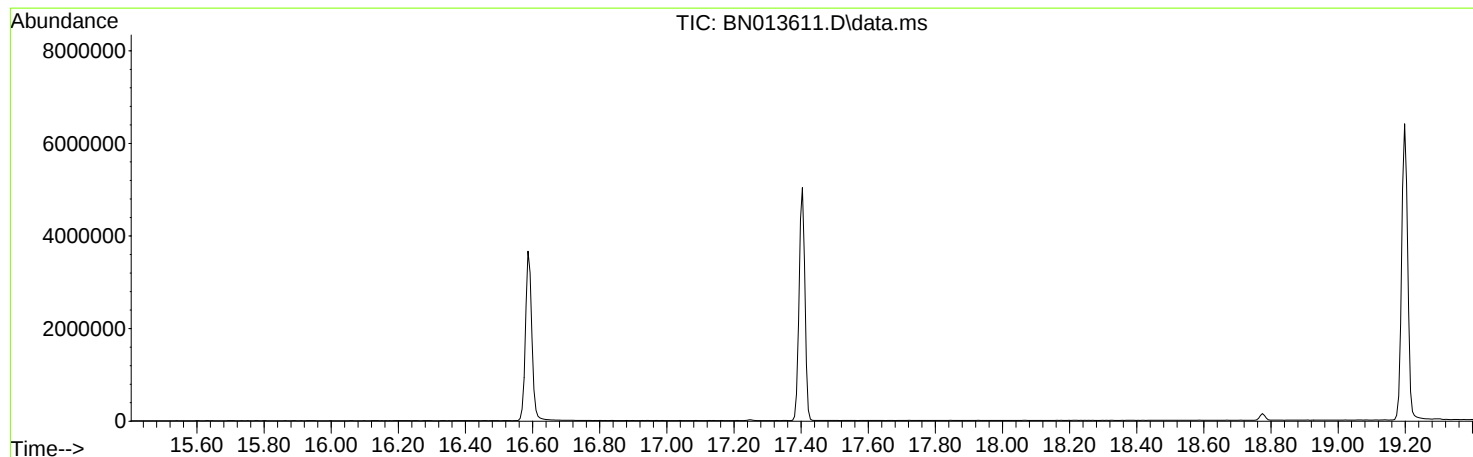

AutoFind: Scans 2433, 2434, 2435; Background Corrected with Scan 2426

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	173456	PASS
68	69	0.00	2	1.9	3294	PASS
69	198	0.00	100	34.9	176237	PASS
70	69	0.00	2	0.5	950	PASS
127	198	10	80	47.2	237803	PASS
197	198	0.00	2	0.2	783	PASS
198	198	100	100	100.0	504299	PASS
199	198	5	9	6.7	33933	PASS
275	198	10	60	25.6	129219	PASS
365	198	1	100	3.2	16042	PASS
441	198	0.01	100	11.5	58029	PASS
442	442	50	100	100.0	452672	PASS
443	442	15	24	18.7	84528	PASS

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/12/2021	BNA_N	<u>BN013611.D</u>
Compound Name	Response	Retention Time
DDT	1779326	20.44
DDD	6892	20
DDE	2195	19.49
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9087	1788413	0.51

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021221\
Data File : BN013611.D
Acq On : 12 Feb 2021 13:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 17 04:28:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 16 05:39:20 2021
Response via : Initial Calibration

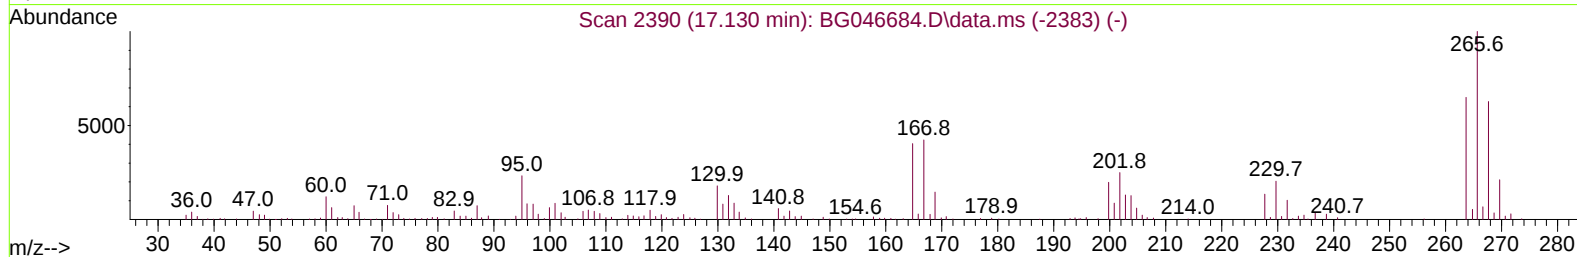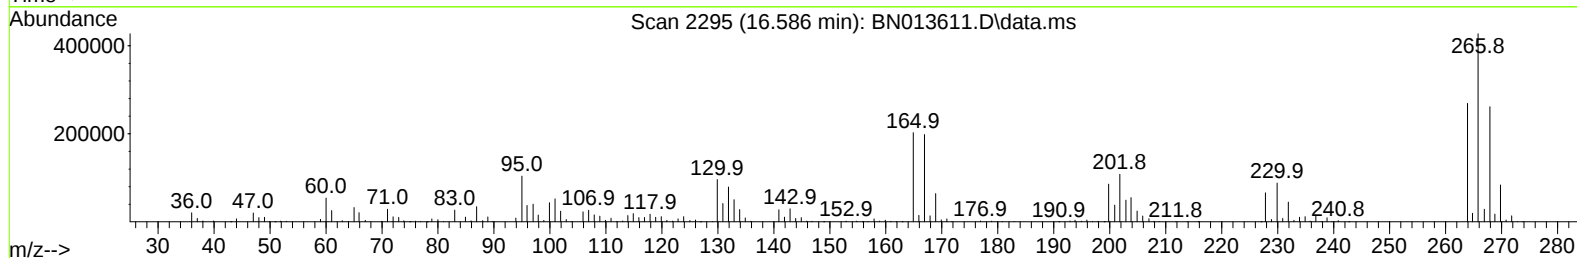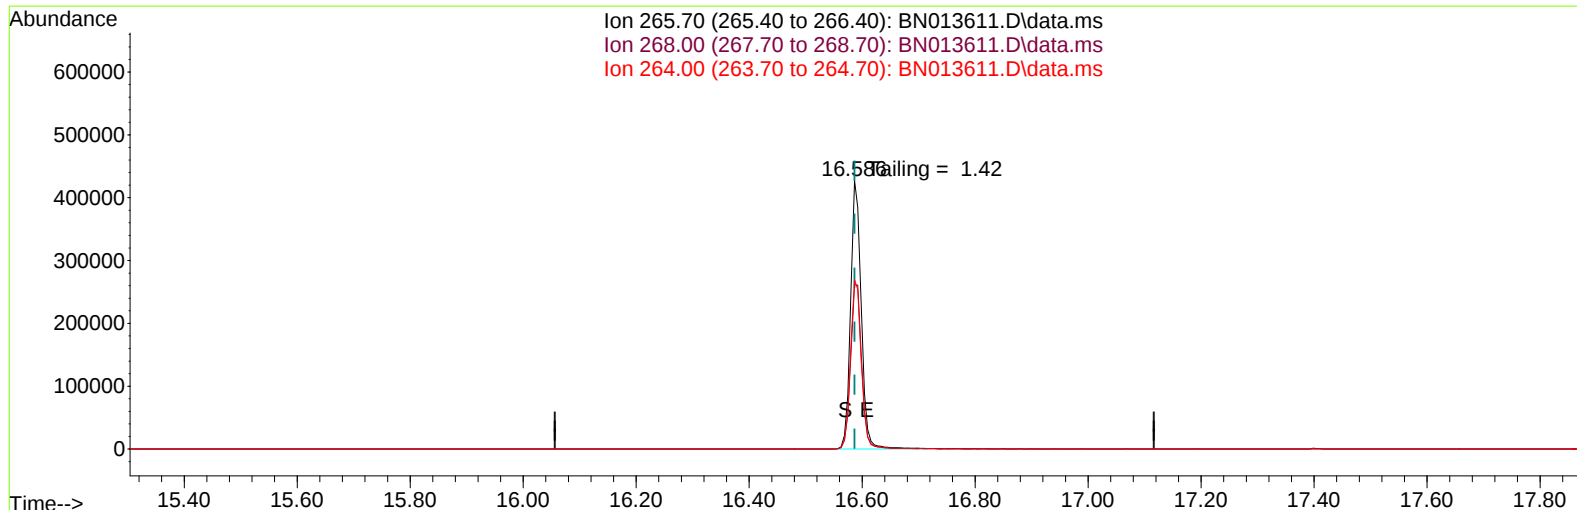

TIC: BN013611.D\data.ms

(70) Pentachlorophenol (C)

16.586min (-0.000) 23509.34 ng




response 563080

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.22
264.00	61.60	63.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021221\
Data File : BN013611.D
Acq On : 12 Feb 2021 13:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 17 04:28:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 16 05:39:20 2021
Response via : Initial Calibration

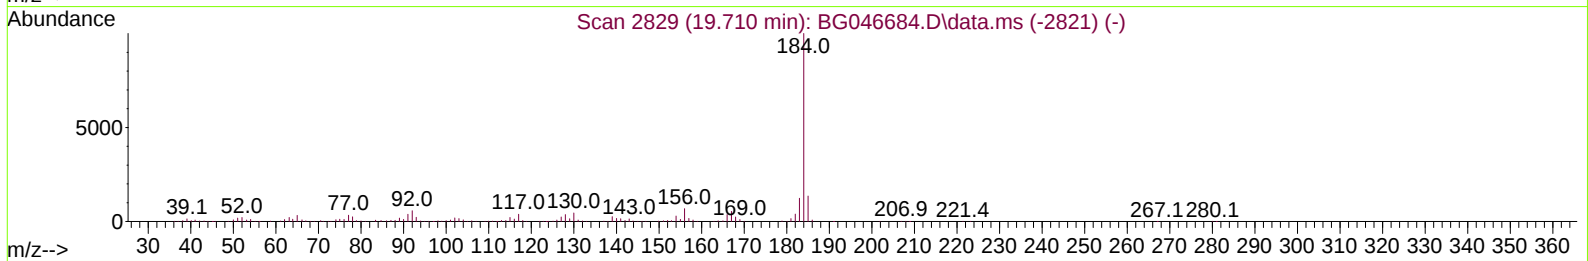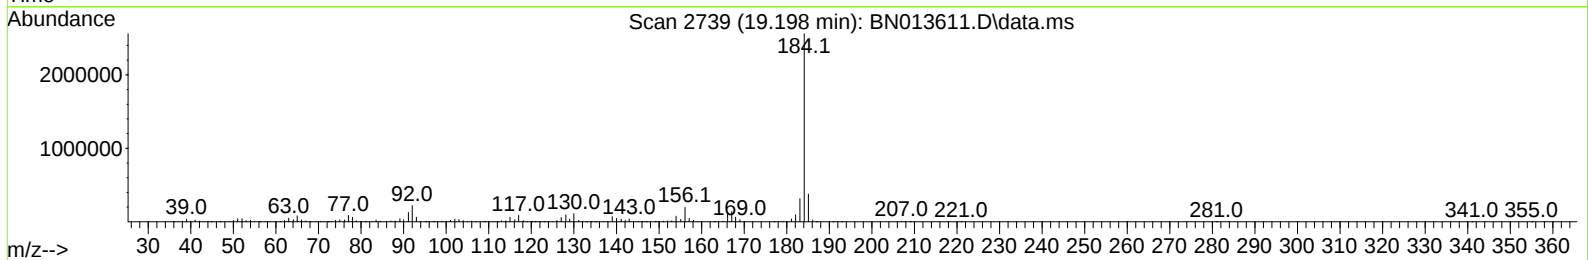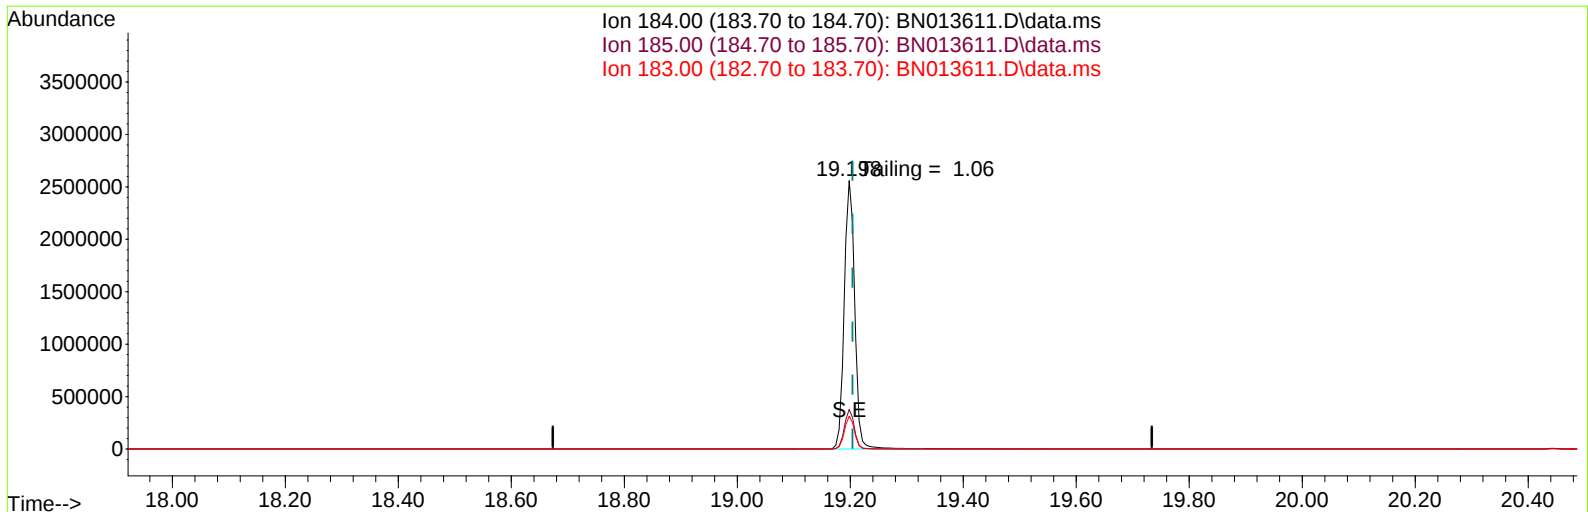

TIC: BN013611.D\data.ms

(77) Benzidine

19.198min (-0.006) 0.00 ng

response 3295620

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.73
183.00	13.20	12.25
0.00	0.00	0.00