




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
 Data File : BN029712.D
 Acq On : 12 Feb 2024 14:11
 Operator : MA/JU
 Sample : P1399-15
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ8

Manual IntegrationsAPPROVED

Quant Time: Feb 12 14:39:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/13/2024
 Supervised By :mohammad ahmed 02/13/2024

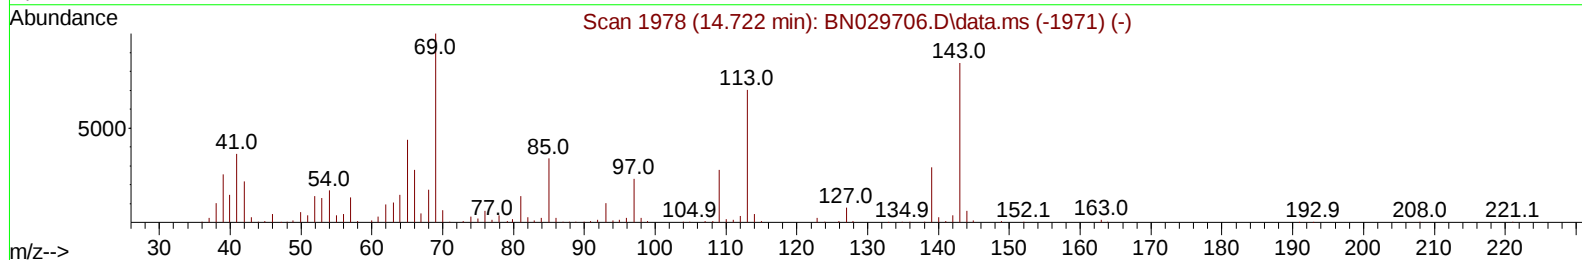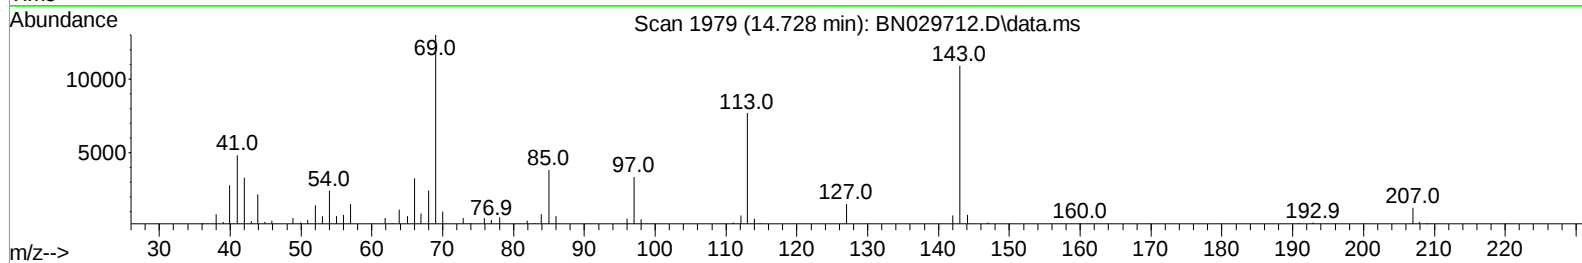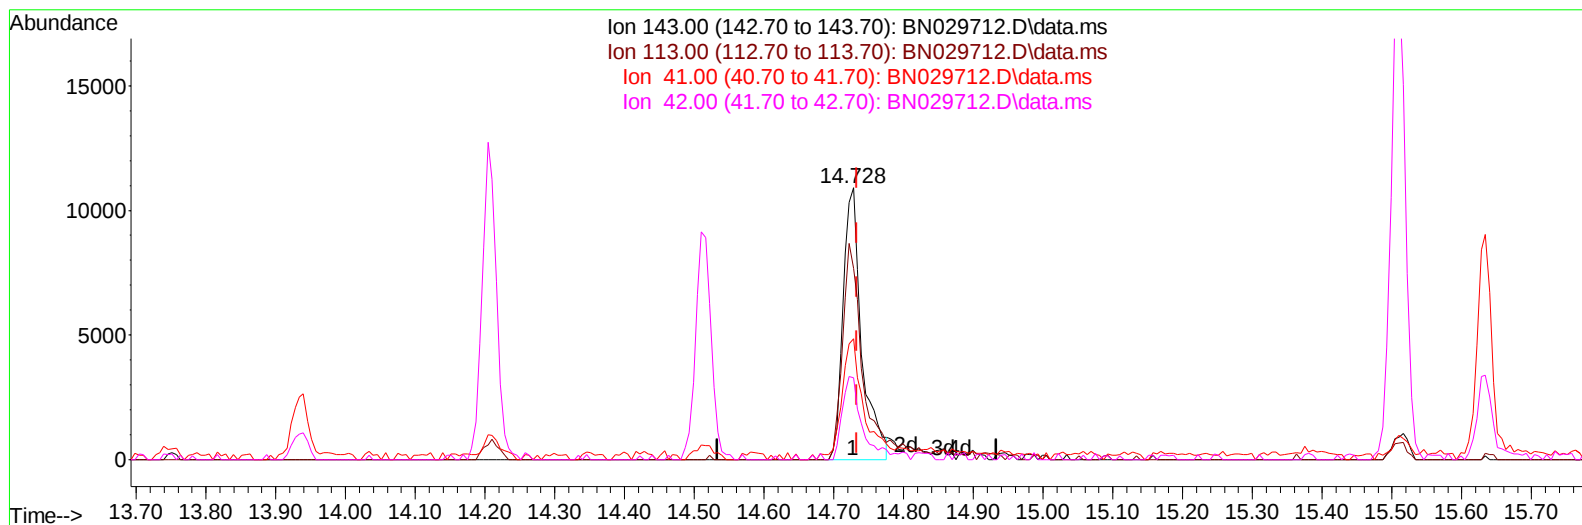

TIC: BN029712.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.728min (-0.006) 3.92 ng/u1

response 20270

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	70.42
41.00	45.90	44.37
42.00	28.40	30.19




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029712.D
Acq On : 12 Feb 2024 14:11
Operator : MA/JU
Sample : P1399-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ8

Manual IntegrationsAPPROVED

Quant Time: Feb 12 14:39:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/13/2024
Supervised By :mohammad ahmed 02/13/2024

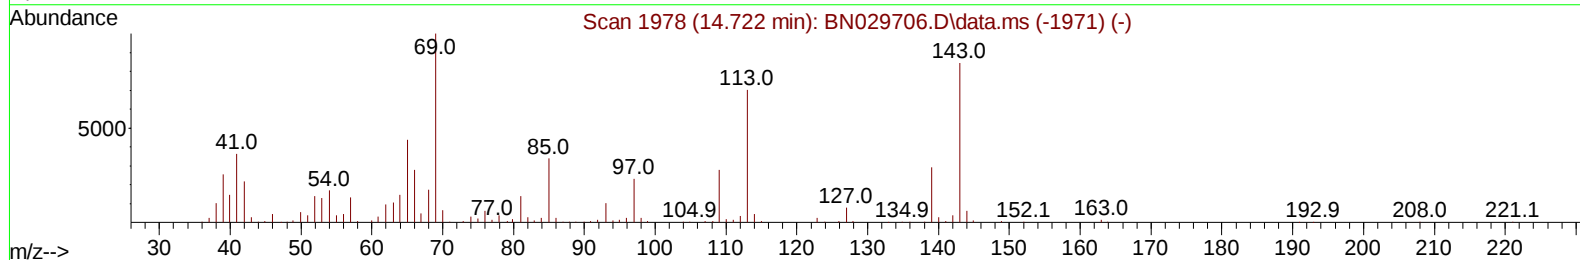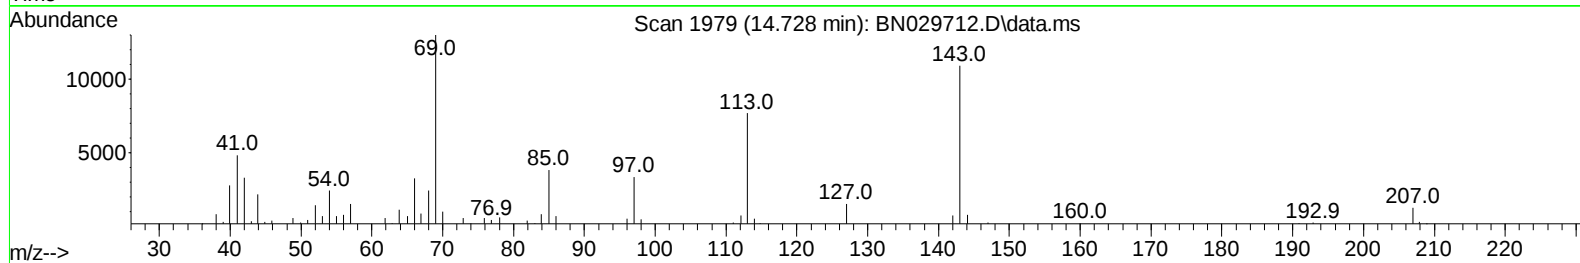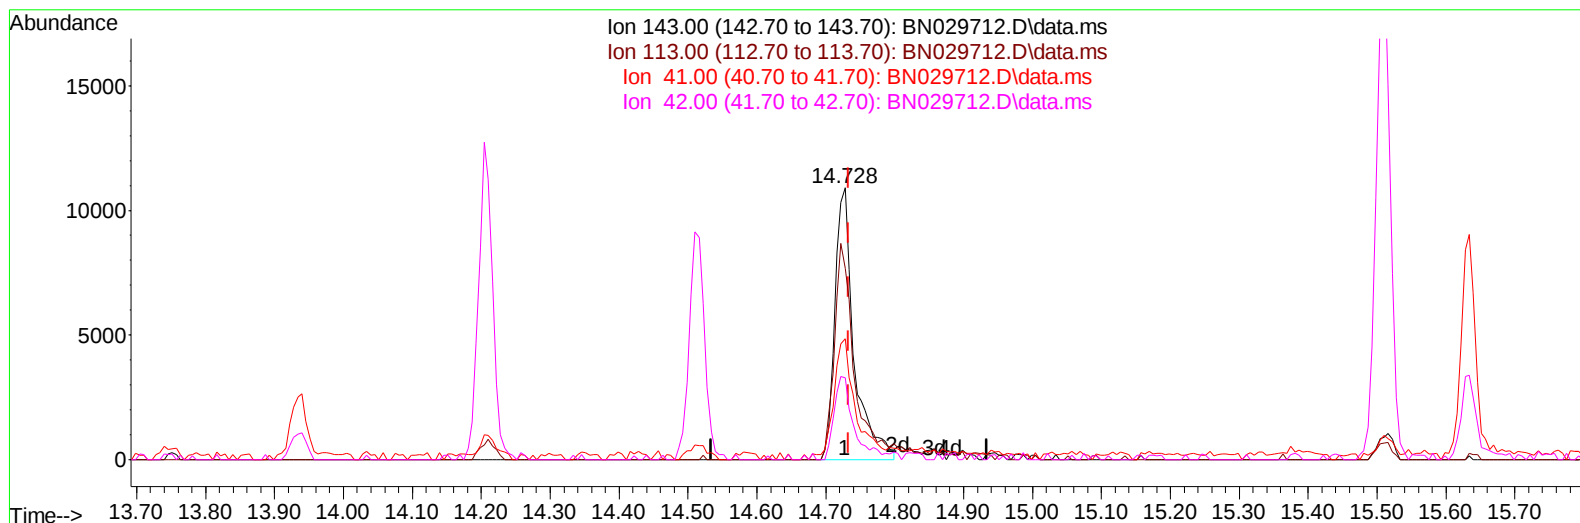

TIC: BN029712.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.728min (-0.006) 4.08 ng/ul m

response 21098

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	87.40	70.42
41.00	45.90	44.37
42.00	28.40	30.19

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
 Data File : BN029712.D
 Acq On : 12 Feb 2024 14:11
 Operator : MA/JU
 Sample : P1399-15
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/13/2024
 Supervised By :mohammad ahmed 02/13/2024

Quant Time: Feb 12 23:13:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 08 00:25:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	194266	20.000	ng/ul	-0.02
20) Naphthalene-d8	10.669	136	766337	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.516	164	366143	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.269	188	645272	20.000	ng/ul	-0.01
79) Chrysene-d12	21.469	240	524412	20.000	ng/ul	-0.01
88) Perylene-d12	23.839	264	622793	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.323	96	26040	4.409	ng/uL	0.00
4) Pyridine-d5	3.740	84	154059	9.781	ng/ul	0.00
7) Phenol-d5	7.040	99	138738	7.635	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.217	67	437084	36.042	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.399	132	388481	29.503	ng/ul	-0.02
15) 4-Methylphenol-d8	8.581	113	214693	15.843	ng/ul	-0.02
21) Nitrobenzene-d5	9.040	128	234231	39.381	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.758	143	209298	40.405	ng/ul	-0.02
28) 2,4-Dichlorophenol-d3	10.293	165	347145	33.952	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.816	131	456086	26.147	ng/ul	-0.02
46) Dimethylphthalate-d6	13.934	166	1085402	39.817	ng/ul	-0.02
49) Acenaphthylene-d8	14.210	160	1242549	38.382	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.728	143	21098m	4.078	ng/ul	0.00
60) Fluorene-d10	15.510	176	902194	38.904	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.634	200	111670	35.517	ng/ul	-0.01
73) Anthracene-d10	17.363	188	1296617	42.876	ng/ul	-0.02
81) Pyrene-d10	19.663	212	1454233	46.210	ng/ul	-0.02
92) Benzo(a)pyrene-d12	23.686	264	1422184	45.636	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029712.D
Acq On : 12 Feb 2024 14:11
Operator : MA/JU
Sample : P1399-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ8

Manual IntegrationsAPPROVED

Quant Time: Feb 12 23:13:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 08 00:25:29 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/13/2024
Supervised By :mohammad ahmed 02/13/2024

