

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
 Data File : BN029707.D
 Acq On : 12 Feb 2024 11:11
 Operator : MA/JU
 Sample : PB158956BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK956

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029707.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	37	40	48	rVB	80720	103566	3.24%	0.229%
2	3.734	106	110	132	rBV	838574	1371636	42.91%	3.026%
3	4.064	161	166	173	rVB	25498	41695	1.30%	0.092%
4	7.040	665	672	686	rBV	1051124	1658504	51.89%	3.659%
5	7.216	695	702	714	rBV	886421	1382394	43.25%	3.050%
6	7.399	726	733	746	rVB	1067285	1676352	52.44%	3.699%
7	7.869	806	813	822	rBV	930051	1468060	45.93%	3.239%
8	8.581	926	934	945	rBV	1223584	1932501	60.46%	4.264%
9	9.040	1005	1012	1025	rBV	936248	1550855	48.52%	3.422%
10	9.758	1126	1134	1149	rBV	693020	1137021	35.57%	2.509%
11	10.216	1211	1212	1217	rBV5	2393	3676	0.12%	0.008%
12	10.287	1217	1224	1240	rVV	1043169	1793559	56.11%	3.957%
13	10.669	1280	1289	1301	rVB	1205501	1990696	62.28%	4.392%
14	10.816	1307	1314	1329	rBV	1054134	1870240	58.51%	4.127%
15	12.263	1555	1560	1570	rBV2	14654	24071	0.75%	0.053%
16	13.422	1751	1757	1762	rVB4	12689	19197	0.60%	0.042%
17	13.934	1838	1844	1856	rBV	1504356	2188445	68.47%	4.829%
18	14.204	1881	1890	1905	rBV2	1840537	2785925	87.16%	6.147%
19	14.387	1918	1921	1927	rVB7	2582	4491	0.14%	0.010%
20	14.516	1936	1943	1955	rBV	1406398	2098072	65.64%	4.629%
21	14.722	1972	1978	1992	rBV	484603	803000	25.12%	1.772%
22	15.510	2102	2112	2122	rBV	2232553	3167075	99.08%	6.988%
23	15.634	2126	2133	2141	rBV	511756	711520	22.26%	1.570%
24	15.751	2148	2153	2159	rVB6	10811	21820	0.68%	0.048%
25	16.075	2204	2208	2211	rBV5	2182	3763	0.12%	0.008%
26	16.298	2241	2246	2252	rVV7	5858	10043	0.31%	0.022%
27	17.057	2370	2375	2378	rBV7	2726	4647	0.15%	0.010%
28	17.263	2404	2410	2421	rBV	1430903	2070700	64.78%	4.569%
29	17.363	2421	2427	2440	rBV2	2084695	3049801	95.41%	6.729%
30	18.539	2624	2627	2631	rBV6	2355	3761	0.12%	0.008%
31	19.233	2740	2745	2750	rBV5	18975	27059	0.85%	0.060%
32	19.304	2752	2757	2761	rBV	17186	26102	0.82%	0.058%
33	19.469	2783	2785	2790	rBV5	4144	6505	0.20%	0.014%
34	19.669	2812	2819	2825	rBV	2202365	3125191	97.77%	6.895%
35	19.881	2853	2855	2859	rBV5	3772	3451	0.11%	0.008%
36	21.469	3119	3125	3132	rBV	1441255	1888657	59.09%	4.167%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029707.D
Acq On : 12 Feb 2024 11:11
Operator : MA/JU
Sample : PB158956BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK956

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	23.686	3495	3502	3517	rBV2	1669623	3196427	100.00%	7.053%
38	23.839	3521	3528	3540	rVB	1027311	2102006	65.76%	4.638%




Sum of corrected areas: 45322484

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029707.D
Acq On : 12 Feb 2024 11:11
Operator : MA/JU
Sample : PB158956BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK956

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

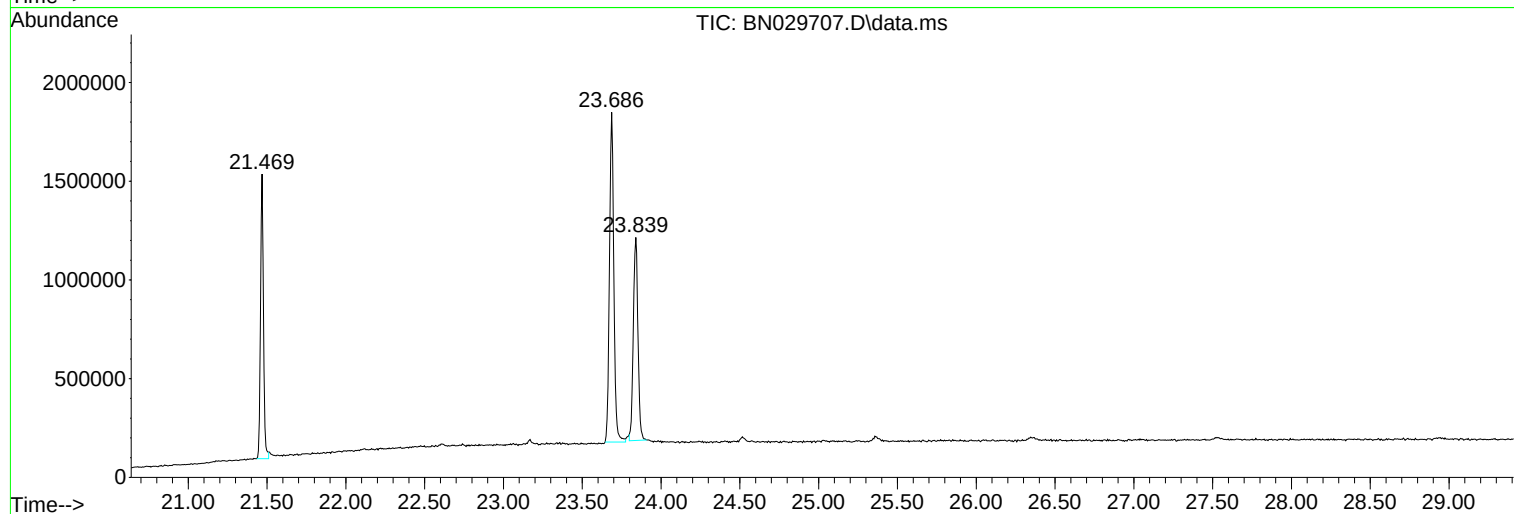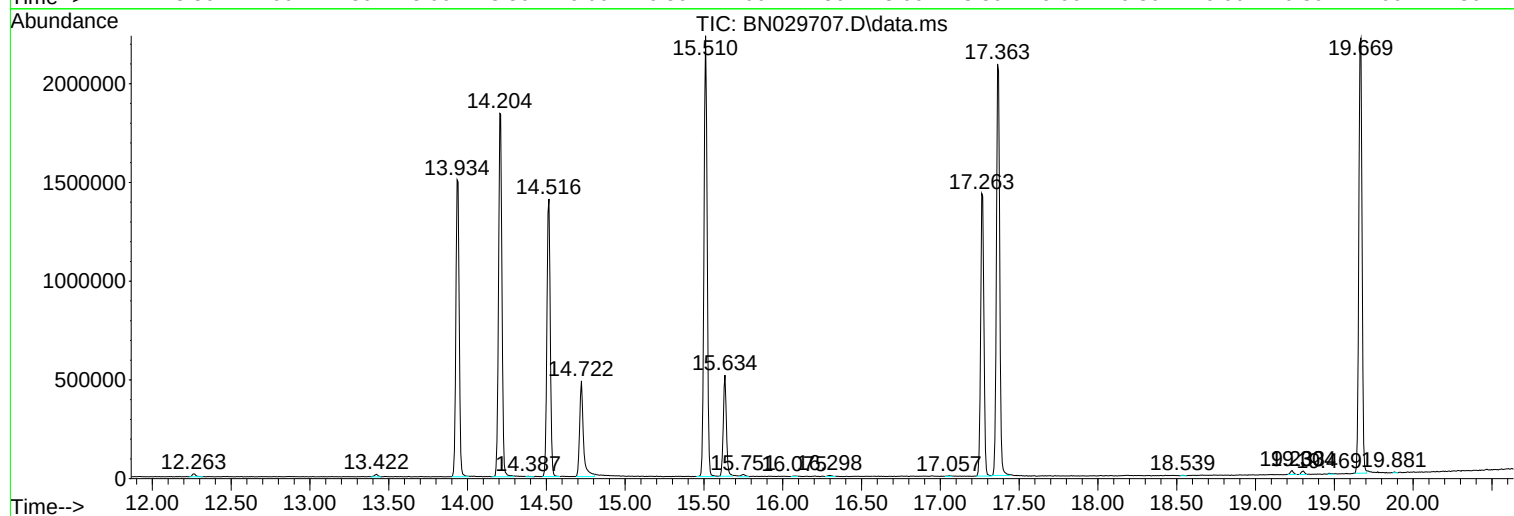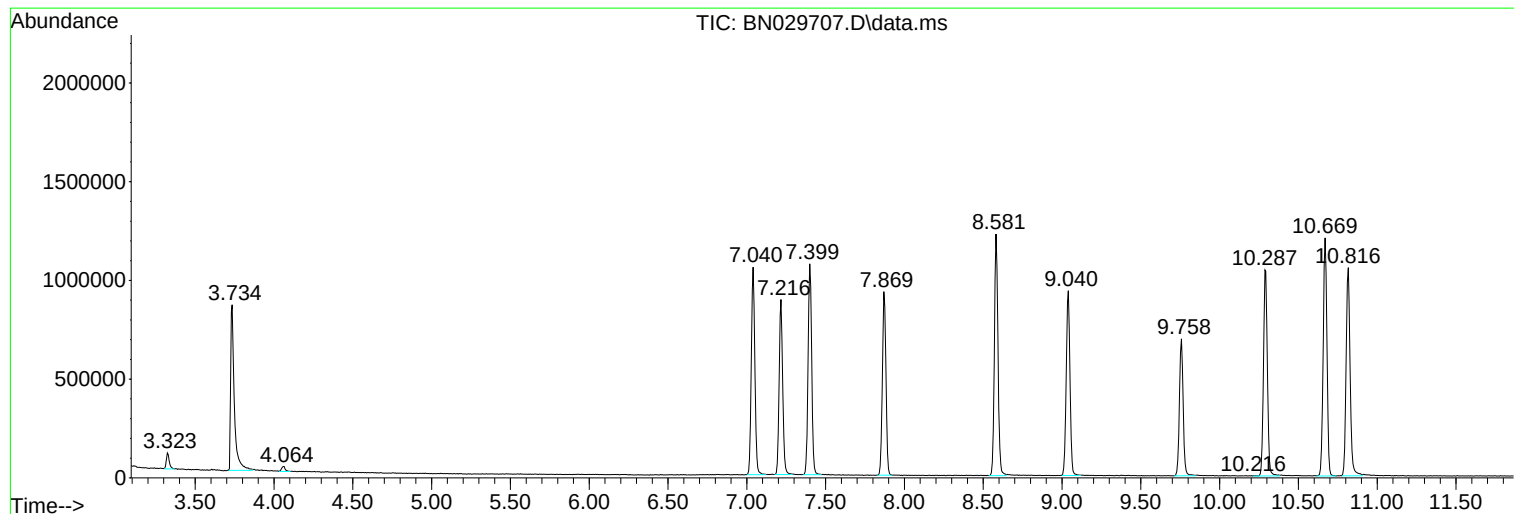

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029707.D
Acq On : 12 Feb 2024 11:11
Operator : MA/JU
Sample : PB158956BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK956

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029707.D
Acq On : 12 Feb 2024 11:11
Operator : MA/JU
Sample : PB158956BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK956

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------