

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
 Data File : BN029708.D
 Acq On : 12 Feb 2024 11:47
 Operator : MA/JU
 Sample : P1399-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	37	40	51	rVB	65511	96576	1.99%	0.177%
2	3.740	108	111	127	rBV	203929	362616	7.46%	0.666%
3	4.058	161	165	174	rVB3	22817	39468	0.81%	0.073%
4	5.005	324	326	330	rVB5	4911	6065	0.12%	0.011%
5	5.158	348	352	357	rVB4	7754	12163	0.25%	0.022%
6	5.881	468	475	478	rBV9	4162	7285	0.15%	0.013%
7	6.958	655	658	662	rVB5	4932	7740	0.16%	0.014%
8	7.040	665	672	683	rBV	343447	541781	11.14%	0.995%
9	7.217	694	702	712	rBV	1280109	2009500	41.32%	3.692%
10	7.399	726	733	744	rBV	1187004	1887523	38.81%	3.468%
11	7.487	746	748	751	rVB4	5001	5353	0.11%	0.010%
12	7.869	804	813	823	rBV	904658	1448683	29.79%	2.662%
13	8.481	910	917	921	rBV7	5629	8318	0.17%	0.015%
14	8.581	927	934	947	rBV	906598	1446725	29.74%	2.658%
15	9.040	1003	1012	1029	rBV	1452420	2352982	48.38%	4.323%
16	9.758	1125	1134	1146	rBV	1032586	1704220	35.04%	3.131%
17	10.293	1216	1225	1238	rBV	1470605	2479342	50.98%	4.555%
18	10.528	1262	1265	1270	rVB7	4771	6645	0.14%	0.012%
19	10.669	1281	1289	1297	rBV	1220508	2015021	41.43%	3.702%
20	10.816	1306	1314	1332	rBV	834292	1468922	30.20%	2.699%
21	11.493	1424	1429	1436	rBV3	18583	36215	0.74%	0.067%
22	12.263	1554	1560	1566	rBV	23553	40718	0.84%	0.075%
23	12.334	1569	1572	1575	rBV4	4681	5802	0.12%	0.011%
24	12.704	1630	1635	1641	rVB3	6439	11541	0.24%	0.021%
25	13.140	1705	1709	1714	rVB4	8216	12003	0.25%	0.022%
26	13.357	1739	1746	1748	rBV6	5352	9431	0.19%	0.017%
27	13.393	1748	1752	1758	rVB4	4911	9391	0.19%	0.017%
28	13.481	1763	1767	1771	rBV7	3917	5995	0.12%	0.011%
29	13.940	1838	1845	1852	rBV	2455286	3500331	71.97%	6.431%
30	14.022	1858	1859	1868	rVB9	2835	5724	0.12%	0.011%
31	14.210	1883	1891	1909	rBV	2918543	4337085	89.17%	7.968%
32	14.516	1936	1943	1950	rBV	1508367	2210837	45.45%	4.062%
33	14.722	1972	1978	1993	rBV	103134	203465	4.18%	0.374%
34	15.510	2103	2112	2117	rBV	3439337	4863794	100.00%	8.936%
35	15.557	2117	2120	2127	rVV	135008	193212	3.97%	0.355%
36	15.634	2127	2133	2143	rVV	885621	1215123	24.98%	2.232%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
 Data File : BN029708.D
 Acq On : 12 Feb 2024 11:47
 Operator : MA/JU
 Sample : P1399-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	15.751	2149	2153	2157	rVB2	15507	24998	0.51%	0.046%
38	16.075	2204	2208	2212	rBV6	3737	5734	0.12%	0.011%
39	16.298	2242	2246	2252	rVB7	10230	14843	0.31%	0.027%
40	16.945	2352	2356	2360	rVB6	4774	7016	0.14%	0.013%
41	17.045	2369	2373	2375	rBV4	3969	5362	0.11%	0.010%
42	17.269	2404	2411	2419	rBV	1472073	2151254	44.23%	3.952%
43	17.369	2421	2428	2439	rBV2	3189505	4713368	96.91%	8.660%
44	17.663	2475	2478	2483	rBV6	5360	8121	0.17%	0.015%
45	18.175	2561	2565	2571	rBV5	24613	38369	0.79%	0.070%
46	18.616	2635	2640	2645	rBV6	10932	15459	0.32%	0.028%
47	19.228	2740	2744	2751	rVB2	34054	47090	0.97%	0.087%
48	19.298	2752	2756	2762	rBV	26467	39061	0.80%	0.072%
49	19.463	2780	2784	2790	rBV4	17618	24813	0.51%	0.046%
50	19.622	2806	2811	2812	rBV4	11327	12461	0.26%	0.023%
51	19.669	2812	2819	2828	rVV	3237122	4591495	94.40%	8.436%
52	21.469	3120	3125	3139	rBV	1350545	1767691	36.34%	3.248%
53	23.686	3495	3502	3515	rBV	2207206	4432697	91.14%	8.144%
54	23.839	3521	3528	3541	rVB	957173	1962463	40.35%	3.605%


Sum of corrected areas: 54429890

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029708.D
Acq On : 12 Feb 2024 11:47
Operator : MA/JU
Sample : P1399-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

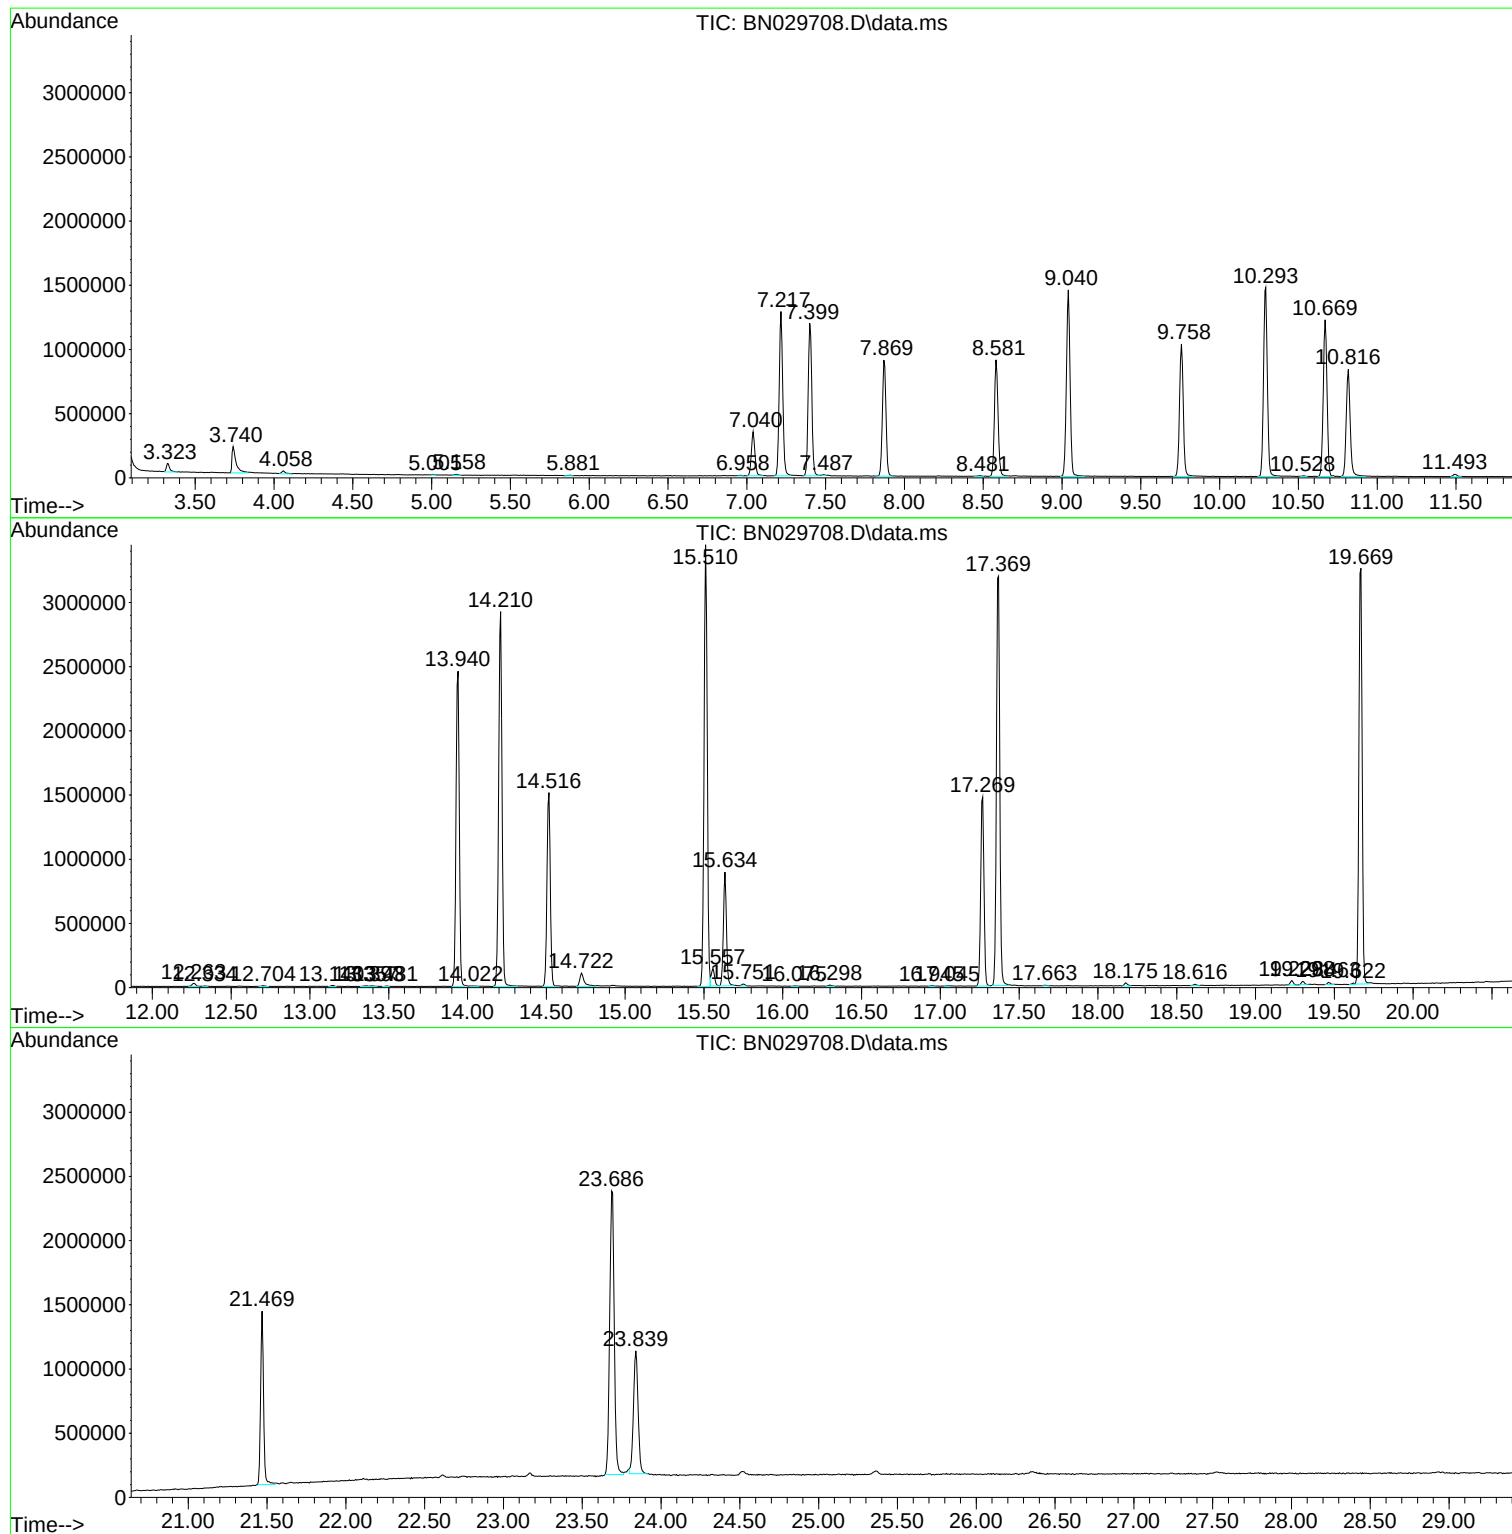

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029708.D
Acq On : 12 Feb 2024 11:47
Operator : MA/JU
Sample : P1399-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029708.D
Acq On : 12 Feb 2024 11:47
Operator : MA/JU
Sample : P1399-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AH5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc