

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
 Data File : BN029710.D
 Acq On : 12 Feb 2024 12:58
 Operator : MA/JU
 Sample : P1399-13
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	37	40	47	rVB	49432	66476	1.57%	0.156%
2	3.740	108	111	128	rBV	144997	260851	6.17%	0.613%
3	4.058	162	165	171	rVB	17448	25305	0.60%	0.059%
4	5.934	481	484	487	rVB5	5237	5969	0.14%	0.014%
5	6.958	655	658	662	rVB4	4766	5617	0.13%	0.013%
6	7.040	665	672	680	rBV	235060	370846	8.78%	0.872%
7	7.216	693	702	720	rBV	917056	1449586	34.30%	3.408%
8	7.399	726	733	745	rBV	858500	1356141	32.09%	3.188%
9	7.487	745	748	750	rBV4	4319	5406	0.13%	0.013%
10	7.869	807	813	821	rBV	744868	1205813	28.53%	2.835%
11	8.581	927	934	945	rBV	627067	1006280	23.81%	2.365%
12	9.040	1004	1012	1027	rBV	1001540	1629851	38.57%	3.831%
13	9.434	1076	1079	1083	rVB6	3311	4698	0.11%	0.011%
14	9.757	1126	1134	1146	rBV	708964	1153170	27.29%	2.711%
15	10.293	1217	1225	1242	rBV	1001007	1690090	39.99%	3.973%
16	10.669	1281	1289	1299	rVB	947243	1591502	37.66%	3.741%
17	10.816	1304	1314	1329	rBV	930997	1642225	38.86%	3.860%
18	12.263	1553	1560	1565	rBV4	14984	26404	0.62%	0.062%
19	13.422	1751	1757	1762	rBV4	13127	21915	0.52%	0.052%
20	13.940	1838	1845	1856	rBV	1638982	2376553	56.24%	5.587%
21	14.210	1884	1891	1900	rBV	1939662	2880394	68.16%	6.771%
22	14.516	1935	1943	1952	rBV	1149333	1682305	39.81%	3.955%
23	14.722	1972	1978	1988	rBV	77145	150730	3.57%	0.354%
24	14.945	2011	2016	2018	rBV4	7156	9978	0.24%	0.023%
25	15.510	2104	2112	2124	rBV	2433920	3460294	81.88%	8.134%
26	15.634	2127	2133	2144	rBV	694755	945166	22.37%	2.222%
27	15.745	2149	2152	2158	rVB4	11958	18618	0.44%	0.044%
28	16.304	2241	2247	2250	rVB6	6756	11398	0.27%	0.027%
29	16.681	2304	2311	2318	rBV8	12019	20825	0.49%	0.049%
30	17.051	2372	2374	2379	rVB6	3586	5003	0.12%	0.012%
31	17.269	2403	2411	2419	rBV	1174359	1666497	39.43%	3.917%
32	17.369	2421	2428	2440	rBV2	2695486	3849064	91.08%	9.048%
33	17.669	2474	2479	2484	rBV6	11955	21171	0.50%	0.050%
34	18.175	2561	2565	2574	rBV	51044	79180	1.87%	0.186%
35	18.480	2613	2617	2621	rBV6	5330	9585	0.23%	0.023%
36	18.616	2636	2640	2644	rBV3	16960	22482	0.53%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029710.D
Acq On : 12 Feb 2024 12:58
Operator : MA/JU
Sample : P1399-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.116	2723	2725	2728	rVB4	5443	5500	0.13%	0.013%
38	19.233	2740	2745	2750	rBV3	28028	41001	0.97%	0.096%
39	19.298	2752	2756	2762	rBV	25249	37464	0.89%	0.088%
40	19.463	2780	2784	2792	rBV2	51715	76091	1.80%	0.179%
41	19.669	2812	2819	2827	rBV	2987663	4093138	96.85%	9.622%
42	21.469	3120	3125	3139	rBV	1194602	1602361	37.92%	3.767%
43	23.686	3495	3502	3515	rBV2	2128685	4226051	100.00%	9.934%
44	23.839	3522	3528	3537	rVB	850458	1731340	40.97%	4.070%


Sum of corrected areas: 42540334

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029710.D
Acq On : 12 Feb 2024 12:58
Operator : MA/JU
Sample : P1399-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

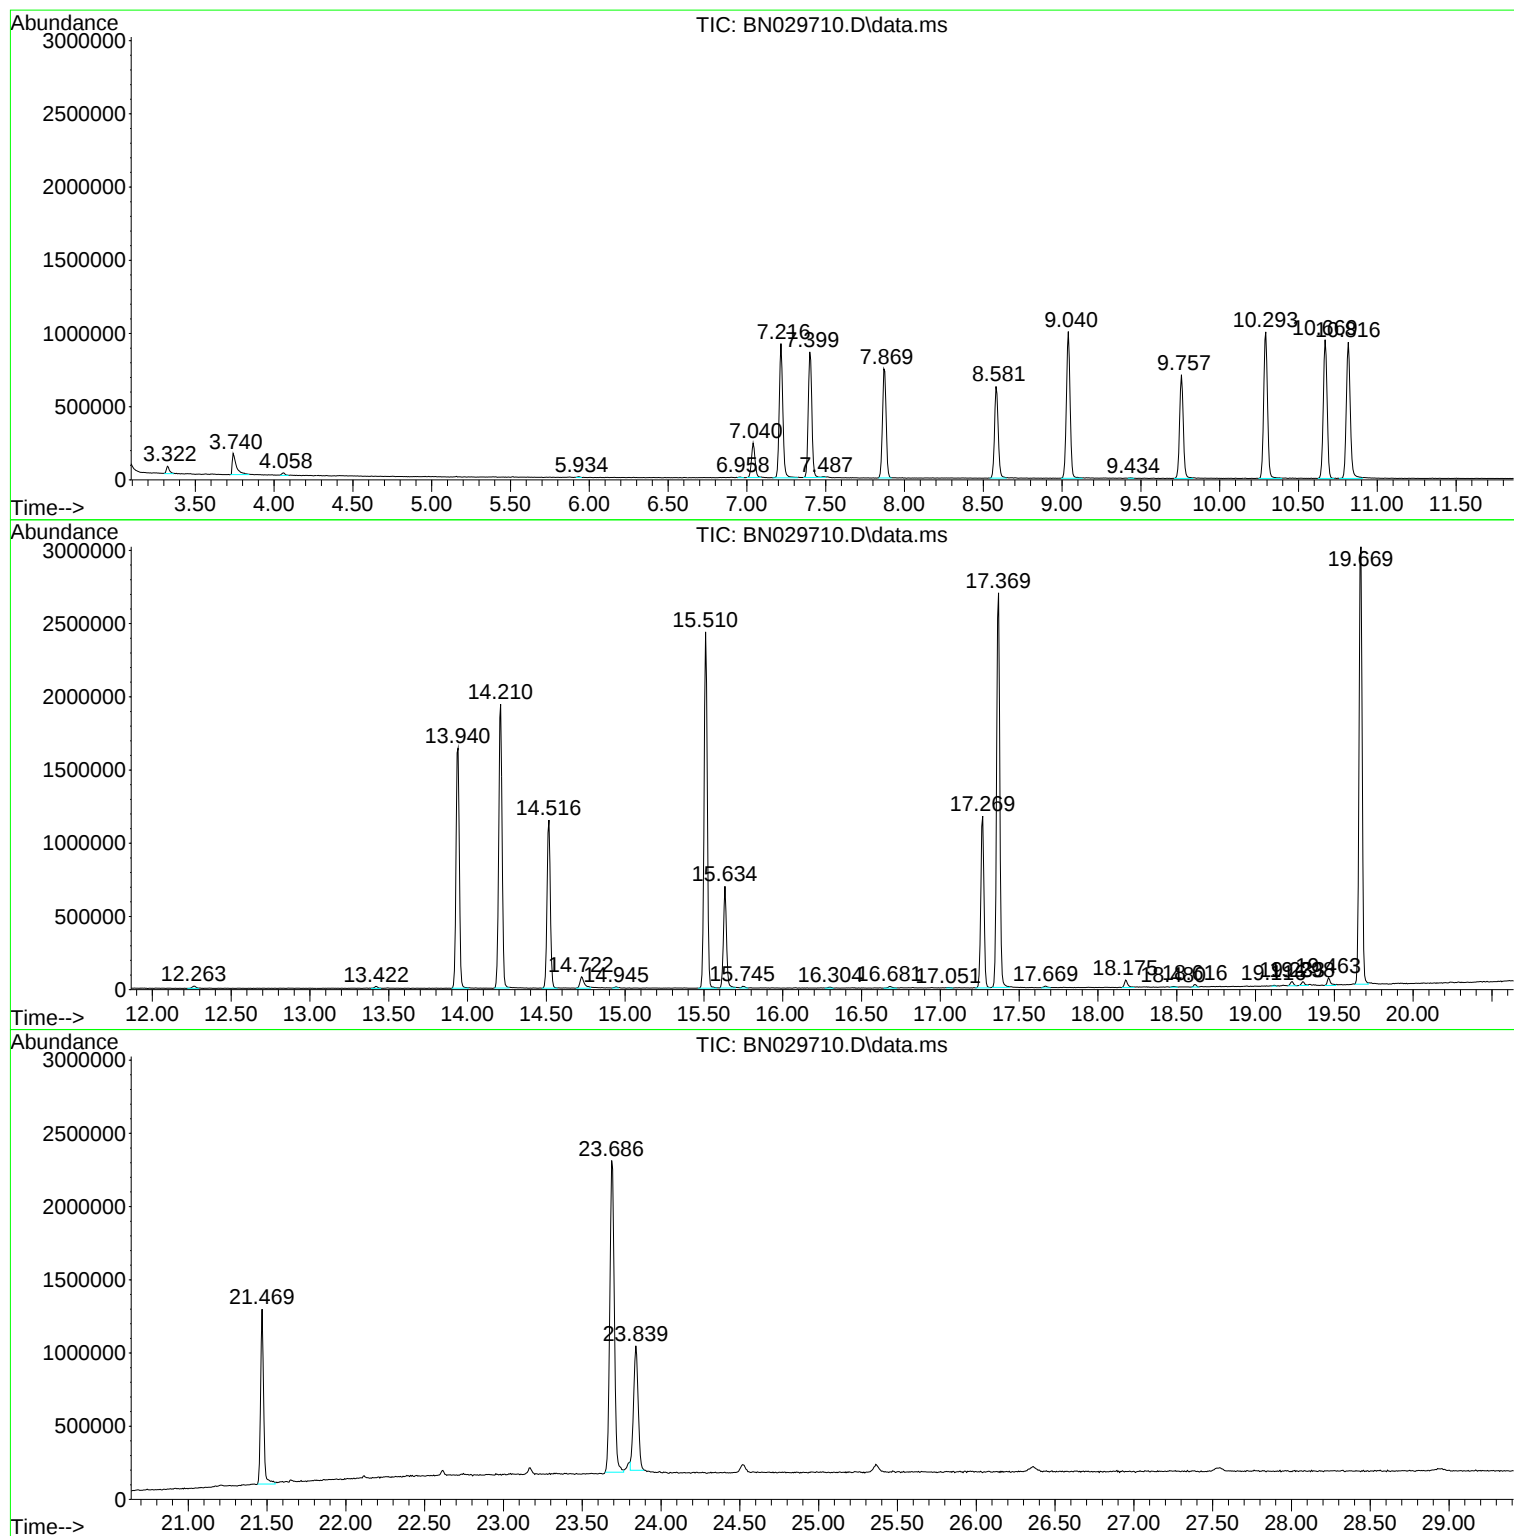

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029710.D
Acq On : 12 Feb 2024 12:58
Operator : MA/JU
Sample : P1399-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029710.D
Acq On : 12 Feb 2024 12:58
Operator : MA/JU
Sample : P1399-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc