

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
 Data File : BN029712.D
 Acq On : 12 Feb 2024 14:11
 Operator : MA/JU
 Sample : P1399-15
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	37	40	51	rVB	55909	86821	2.04%	0.197%
2	3.740	108	111	126	rBV	244050	427749	10.07%	0.972%
3	4.058	161	165	172	rVB	16913	23652	0.56%	0.054%
4	5.158	346	352	359	rBV	59206	88661	2.09%	0.201%
5	6.958	652	658	661	rVB6	4040	5812	0.14%	0.013%
6	7.040	666	672	678	rBV	262195	397655	9.36%	0.904%
7	7.217	695	702	714	rBV	949987	1508530	35.51%	3.428%
8	7.399	726	733	744	rBV	896948	1422629	33.48%	3.233%
9	7.869	806	813	820	rBV	770275	1224904	28.83%	2.783%
10	8.581	927	934	949	rBV	599093	956740	22.52%	2.174%
11	9.040	1004	1012	1021	rBV	1049144	1710700	40.26%	3.887%
12	9.758	1127	1134	1148	rBV	733855	1232861	29.02%	2.801%
13	10.293	1217	1225	1237	rBV	1055546	1793424	42.21%	4.075%
14	10.669	1281	1289	1298	rBV	973064	1633902	38.46%	3.713%
15	10.816	1306	1314	1326	rBV	870956	1526842	35.94%	3.470%
16	11.493	1423	1429	1435	rBV	46339	78563	1.85%	0.179%
17	12.263	1554	1560	1567	rBV2	16198	28605	0.67%	0.065%
18	13.416	1752	1756	1764	rVB	10086	16042	0.38%	0.036%
19	13.746	1809	1812	1819	rVB7	5676	9091	0.21%	0.021%
20	13.934	1837	1844	1854	rBV	1776931	2518321	59.27%	5.722%
21	14.210	1882	1891	1902	rBV	2014963	3028797	71.29%	6.882%
22	14.516	1935	1943	1950	rBV	1173855	1731496	40.75%	3.935%
23	14.722	1973	1978	1991	rBV	79221	166071	3.91%	0.377%
24	14.934	2012	2014	2017	rBV4	3368	4362	0.10%	0.010%
25	15.375	2086	2089	2096	rVB9	5032	9030	0.21%	0.021%
26	15.510	2105	2112	2119	rBV	2589061	3645432	85.80%	8.284%
27	15.634	2126	2133	2142	rBV	702456	949097	22.34%	2.157%
28	15.751	2147	2153	2159	rVB5	10778	18052	0.42%	0.041%
29	16.245	2233	2237	2242	rVV6	4616	7917	0.19%	0.018%
30	16.298	2242	2246	2249	rVB4	6399	8617	0.20%	0.020%
31	16.816	2329	2334	2338	rVB7	3256	5421	0.13%	0.012%
32	17.040	2368	2372	2378	rBV5	5858	12370	0.29%	0.028%
33	17.269	2404	2411	2421	rBV	1190052	1720412	40.49%	3.909%
34	17.363	2421	2427	2442	rVV2	2430220	3641818	85.71%	8.275%
35	17.663	2471	2478	2480	rBV6	5313	8074	0.19%	0.018%
36	17.775	2495	2497	2503	rBV7	5572	9773	0.23%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
 Data File : BN029712.D
 Acq On : 12 Feb 2024 14:11
 Operator : MA/JU
 Sample : P1399-15
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	17.957	2522	2528	2534	rBV	49769	69131	1.63%	0.157%
38	18.175	2561	2565	2571	rBV2	35474	54282	1.28%	0.123%
39	18.498	2614	2620	2625	rBV8	10113	23606	0.56%	0.054%
40	18.610	2636	2639	2643	rBV5	5847	7595	0.18%	0.017%
41	18.657	2643	2647	2654	rVB5	16297	25967	0.61%	0.059%
42	19.110	2719	2724	2726	rBV3	20211	28106	0.66%	0.064%
43	19.139	2726	2729	2733	rVV2	65661	74143	1.75%	0.168%
44	19.234	2740	2745	2748	rVB	29074	38643	0.91%	0.088%
45	19.275	2748	2752	2753	rBV	21051	21525	0.51%	0.049%
46	19.298	2753	2756	2761	rVB	31270	43045	1.01%	0.098%
47	19.463	2780	2784	2790	rBV4	17071	23141	0.54%	0.053%
48	19.616	2807	2810	2812	rBV4	7112	9080	0.21%	0.021%
49	19.663	2812	2818	2827	rVV	2945197	4107447	96.67%	9.334%
50	19.928	2860	2863	2867	rVB3	28410	33040	0.78%	0.075%
51	21.198	3076	3079	3084	rVB6	21970	30983	0.73%	0.070%
52	21.469	3119	3125	3134	rBV	1255515	1651244	38.86%	3.752%
53	23.686	3494	3502	3516	rBV2	2097569	4248767	100.00%	9.655%
54	23.839	3521	3528	3538	rVB	935316	1859428	43.76%	4.225%




Sum of corrected areas: 44007416

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029712.D
Acq On : 12 Feb 2024 14:11
Operator : MA/JU
Sample : P1399-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

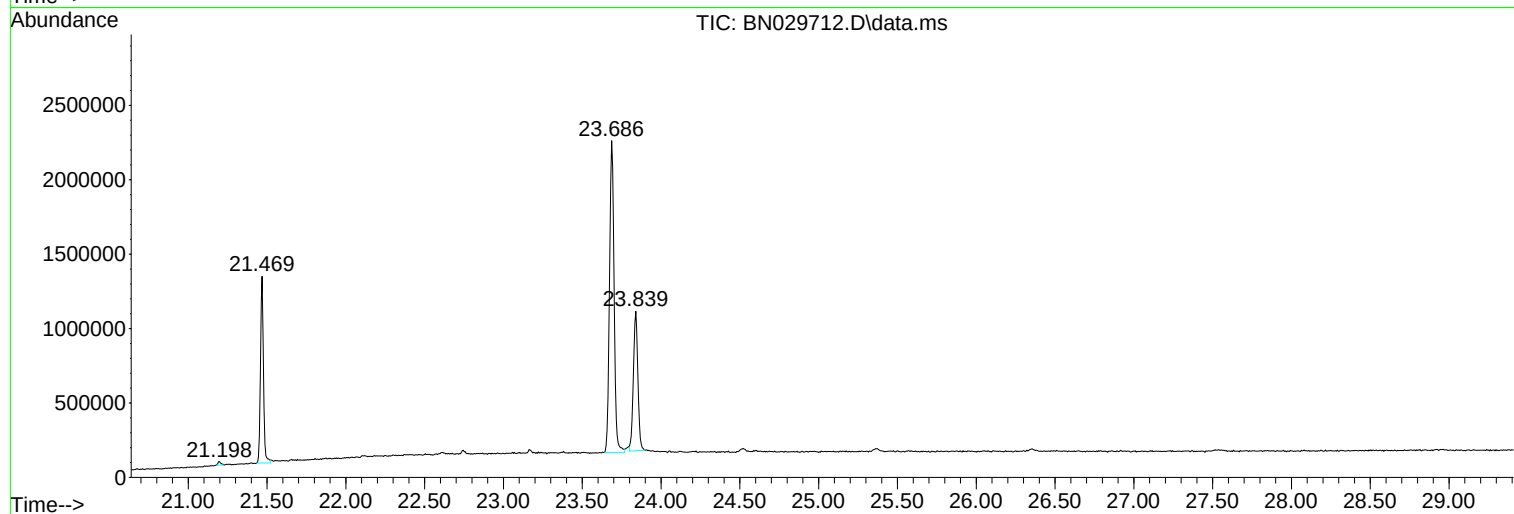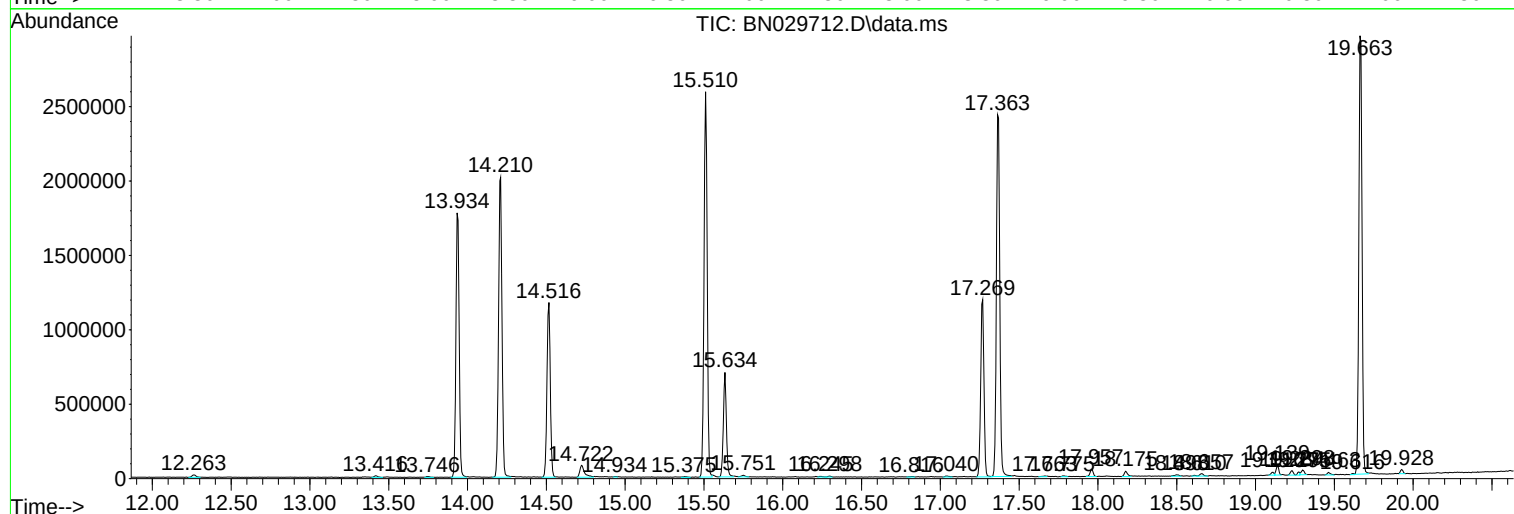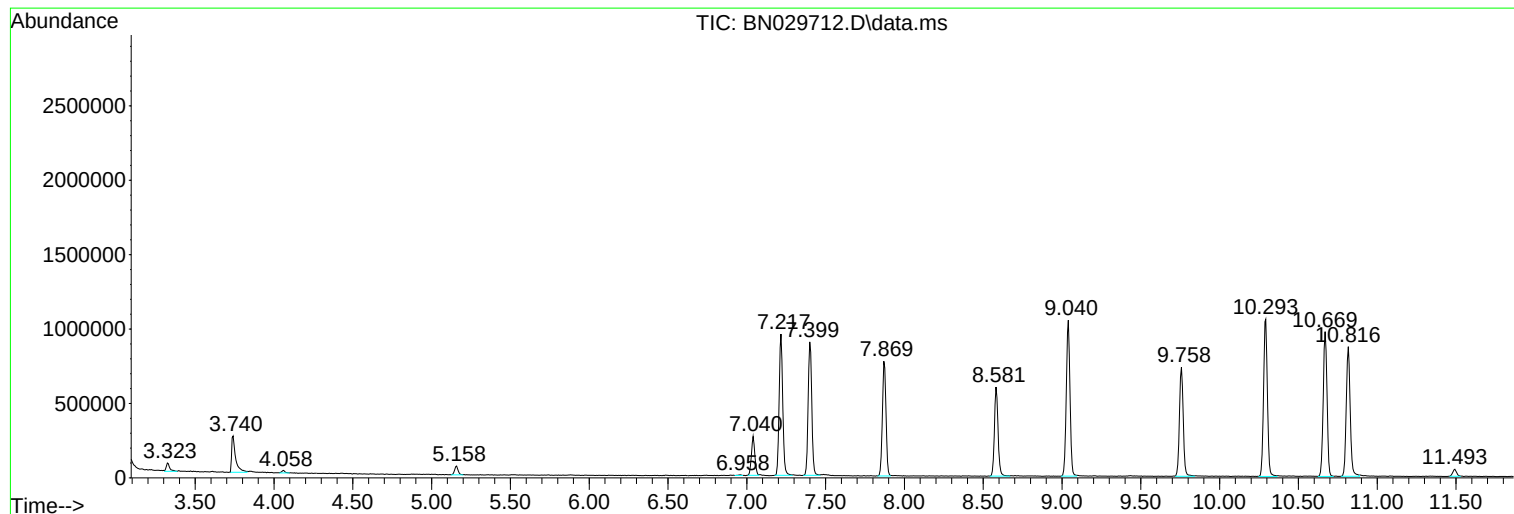

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029712.D
Acq On : 12 Feb 2024 14:11
Operator : MA/JU
Sample : P1399-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029712.D
Acq On : 12 Feb 2024 14:11
Operator : MA/JU
Sample : P1399-15
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc