

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
 Data File : BN029713.D
 Acq On : 12 Feb 2024 14:47
 Operator : MA/JU
 Sample : P1402-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	37	40	49	rVB	55672	76998	1.97%	0.175%
2	3.740	107	111	127	rBV	263338	468674	12.00%	1.064%
3	4.057	161	165	171	rVB	15740	24439	0.63%	0.055%
4	5.534	409	416	421	rBV	40390	63417	1.62%	0.144%
5	7.040	665	672	687	rVB	228138	366102	9.38%	0.831%
6	7.216	695	702	714	rBV	1048243	1639825	42.00%	3.722%
7	7.398	726	733	744	rBV	896911	1427987	36.57%	3.241%
8	7.481	745	747	753	rVB6	4782	7462	0.19%	0.017%
9	7.869	806	813	823	rVV	762361	1223971	31.35%	2.778%
10	8.581	927	934	946	rBV	602166	974594	24.96%	2.212%
11	9.040	1004	1012	1019	rBV	1148645	1852651	47.45%	4.205%
12	9.428	1073	1078	1084	rVB4	8628	14922	0.38%	0.034%
13	9.622	1108	1111	1116	rBV7	5646	7823	0.20%	0.018%
14	9.757	1127	1134	1149	rVV	790532	1300932	33.32%	2.953%
15	10.292	1217	1225	1243	rBV	1121168	1885276	48.29%	4.279%
16	10.669	1282	1289	1299	rVB	980206	1631947	41.80%	3.704%
17	10.816	1306	1314	1326	rBV	929873	1604937	41.11%	3.642%
18	11.428	1411	1418	1426	rBV2	13791	32640	0.84%	0.074%
19	11.492	1426	1429	1439	rVB9	5061	10934	0.28%	0.025%
20	12.263	1554	1560	1566	rBV	19839	32736	0.84%	0.074%
21	12.475	1591	1596	1601	rVB8	3506	4844	0.12%	0.011%
22	13.145	1705	1710	1714	rVB6	3724	5961	0.15%	0.014%
23	13.351	1741	1745	1748	rBV4	5766	6882	0.18%	0.016%
24	13.416	1751	1756	1762	rVB3	17132	27170	0.70%	0.062%
25	13.939	1838	1845	1858	rBV	1920532	2716653	69.58%	6.166%
26	14.051	1861	1864	1868	rVB5	3227	3992	0.10%	0.009%
27	14.210	1882	1891	1902	rBV	2197000	3312805	84.85%	7.519%
28	14.516	1936	1943	1950	rBV	1183949	1745694	44.71%	3.962%
29	14.727	1973	1979	1990	rBV	61785	131451	3.37%	0.298%
30	15.322	2076	2080	2084	rBV	16551	21322	0.55%	0.048%
31	15.510	2105	2112	2119	rBV	2658798	3823586	97.93%	8.678%
32	15.633	2127	2133	2141	rBV	668640	912347	23.37%	2.071%
33	15.751	2148	2153	2158	rVB4	11390	16127	0.41%	0.037%
34	16.074	2206	2208	2213	rVB5	4174	4623	0.12%	0.010%
35	16.298	2242	2246	2250	rBV5	7840	9121	0.23%	0.021%
36	16.674	2307	2310	2312	rBV3	4707	5704	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
 Data File : BN029713.D
 Acq On : 12 Feb 2024 14:47
 Operator : MA/JU
 Sample : P1402-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	16.945	2352	2356	2361	rVB7	3771	6322	0.16%	0.014%
38	17.045	2369	2373	2375	rBV4	4206	5028	0.13%	0.011%
39	17.263	2400	2410	2417	rBV	1157012	1688388	43.24%	3.832%
40	17.369	2421	2428	2440	rVV	2501016	3655612	93.63%	8.297%
41	17.451	2440	2442	2446	rVB5	6325	6510	0.17%	0.015%
42	17.574	2458	2463	2465	rVB5	4796	5882	0.15%	0.013%
43	17.639	2470	2474	2476	rBV5	6293	7648	0.20%	0.017%
44	17.786	2493	2499	2501	rBV7	2414	5254	0.13%	0.012%
45	17.951	2523	2527	2532	rVB7	5203	7290	0.19%	0.017%
46	18.010	2535	2537	2539	rVV3	4802	4089	0.10%	0.009%
47	18.051	2539	2544	2551	rVB8	5951	10050	0.26%	0.023%
48	18.174	2561	2565	2573	rBV	62322	85590	2.19%	0.194%
49	18.257	2576	2579	2583	rVB5	4858	6625	0.17%	0.015%
50	18.610	2637	2639	2644	rBV5	5110	8098	0.21%	0.018%
51	18.663	2644	2648	2653	rVB8	4735	8151	0.21%	0.018%
52	19.227	2739	2744	2751	rBV	28181	42154	1.08%	0.096%
53	19.298	2751	2756	2761	rBV	28405	48145	1.23%	0.109%
54	19.339	2761	2763	2767	rVB5	6912	8964	0.23%	0.020%
55	19.463	2780	2784	2789	rBV4	19281	26230	0.67%	0.060%
56	19.557	2798	2800	2806	rVB6	10492	12782	0.33%	0.029%
57	19.621	2808	2811	2812	rBV3	7143	5963	0.15%	0.014%
58	19.663	2812	2818	2826	rBV	2778906	3886957	99.55%	8.822%
59	21.198	3076	3079	3085	rBV4	47541	58497	1.50%	0.133%
60	21.468	3119	3125	3134	rBV2	1132847	1499585	38.41%	3.403%
61	23.686	3494	3502	3514	rBV2	1950222	3904460	100.00%	8.861%
62	23.839	3522	3528	3541	rVB	822633	1660740	42.53%	3.769%




Sum of corrected areas: 44061563

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029713.D
Acq On : 12 Feb 2024 14:47
Operator : MA/JU
Sample : P1402-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

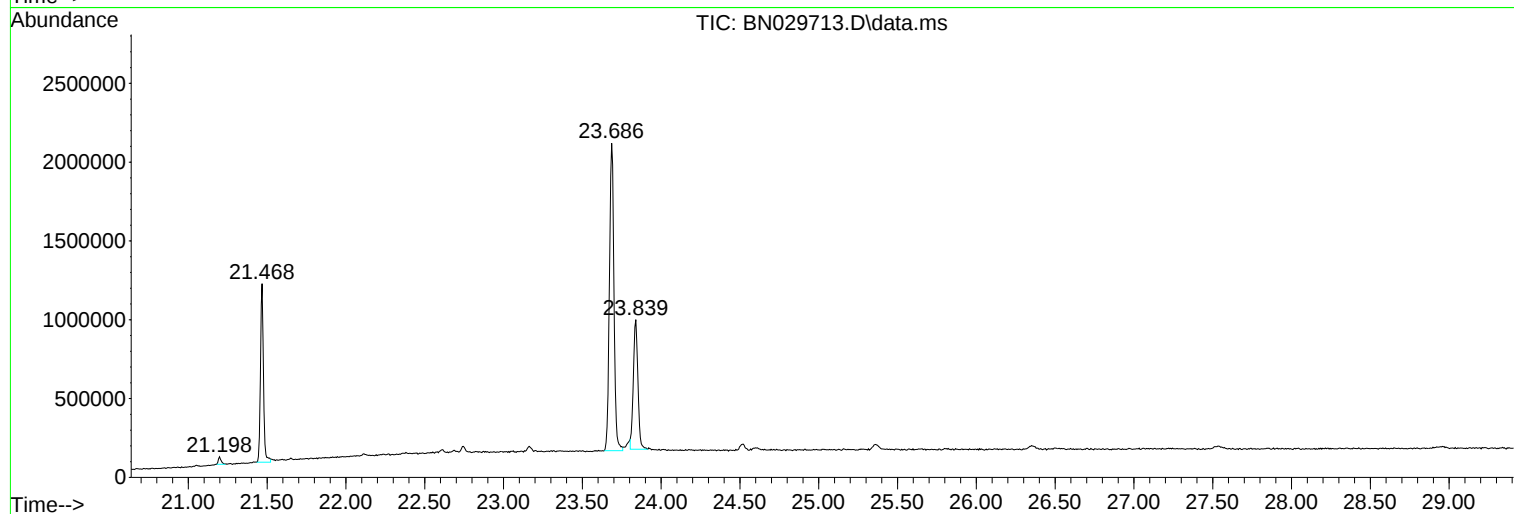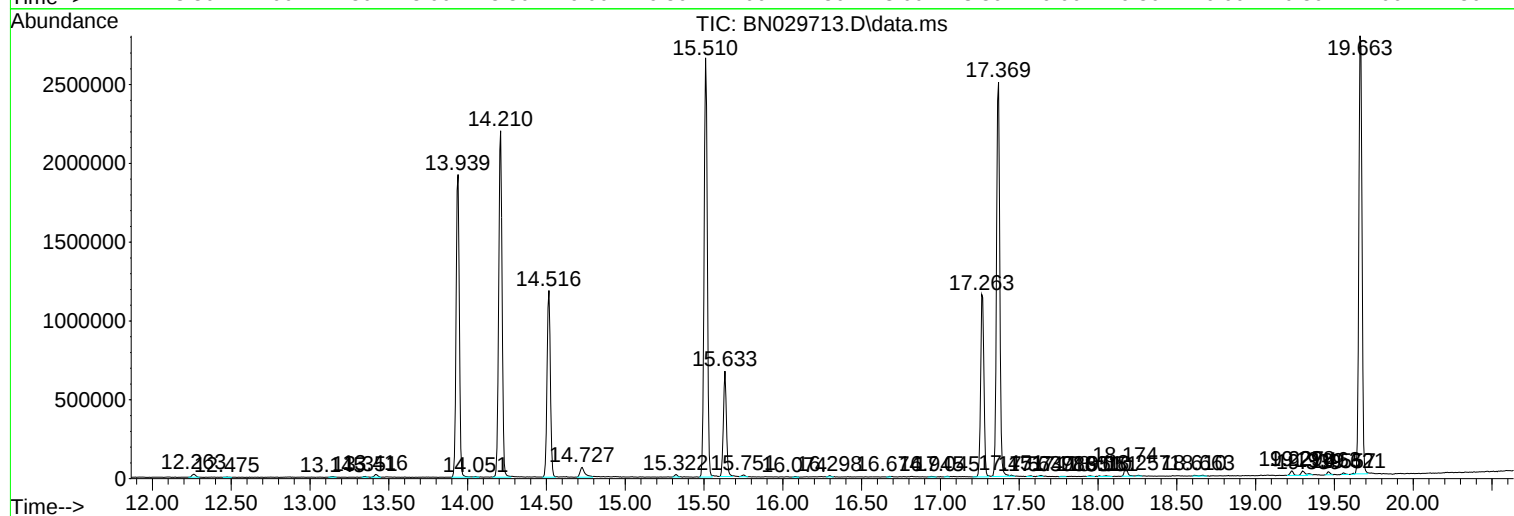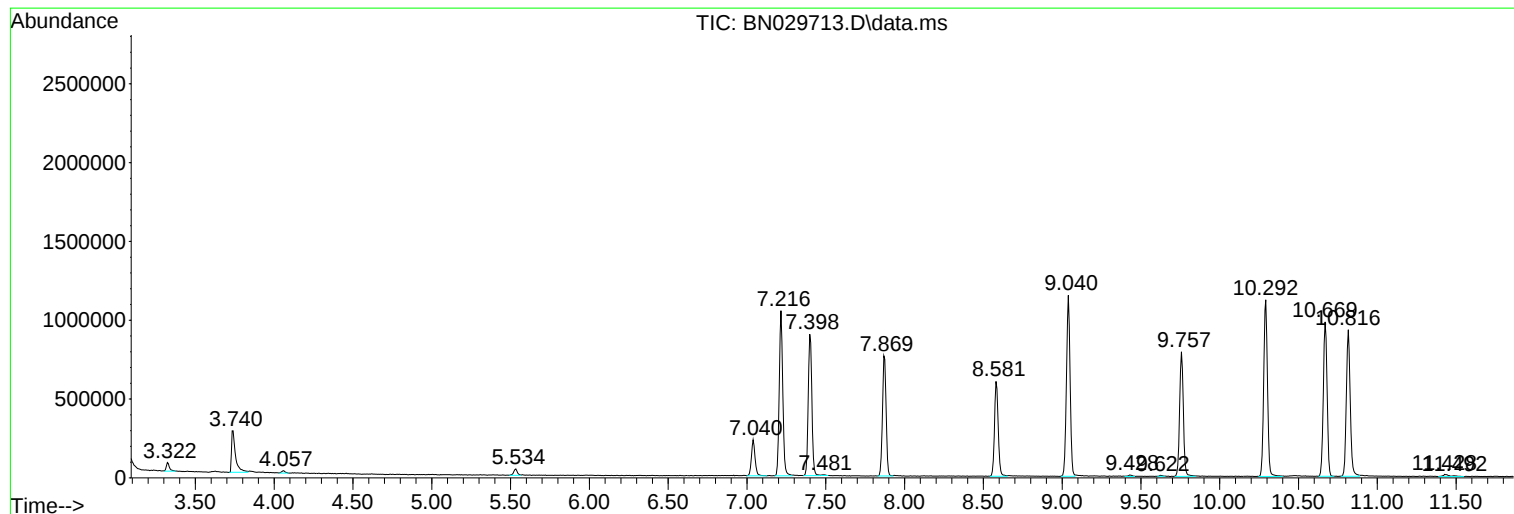

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029713.D
Acq On : 12 Feb 2024 14:47
Operator : MA/JU
Sample : P1402-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021224\
Data File : BN029713.D
Acq On : 12 Feb 2024 14:47
Operator : MA/JU
Sample : P1402-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc