
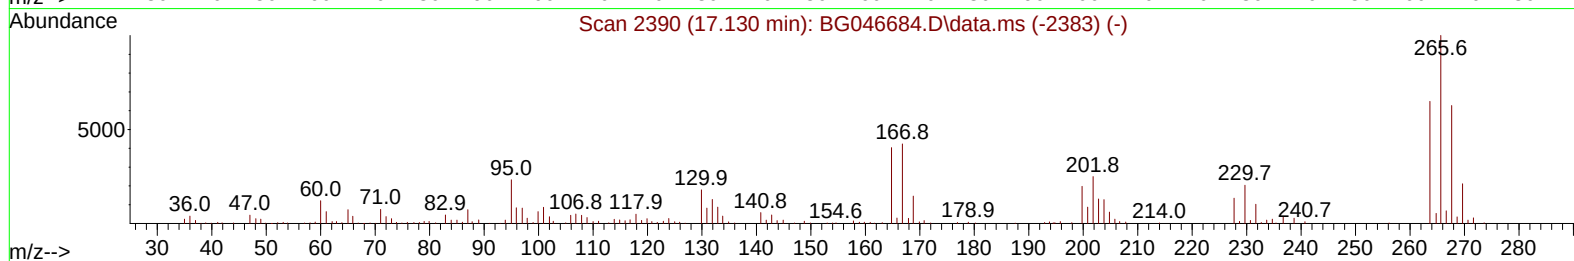
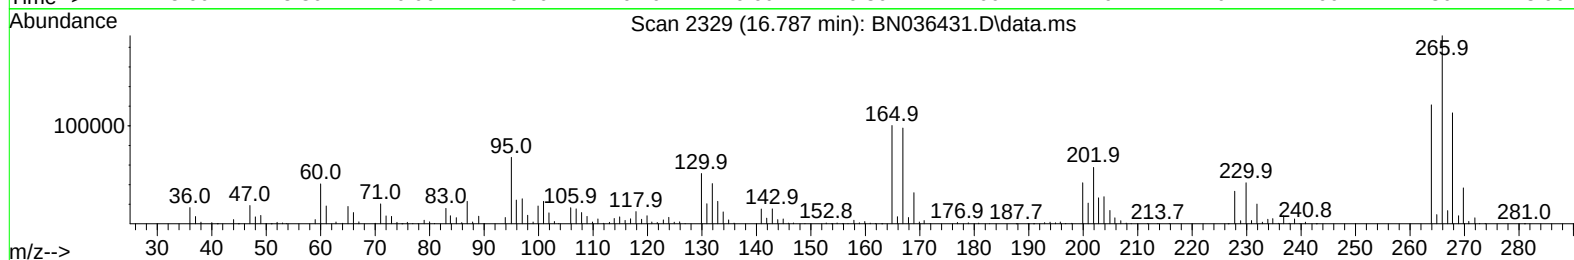


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021225\
Data File : BN036431.D
Acq On : 12 Feb 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 14:50:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 14:47:47 2025
Response via : Initial Calibration

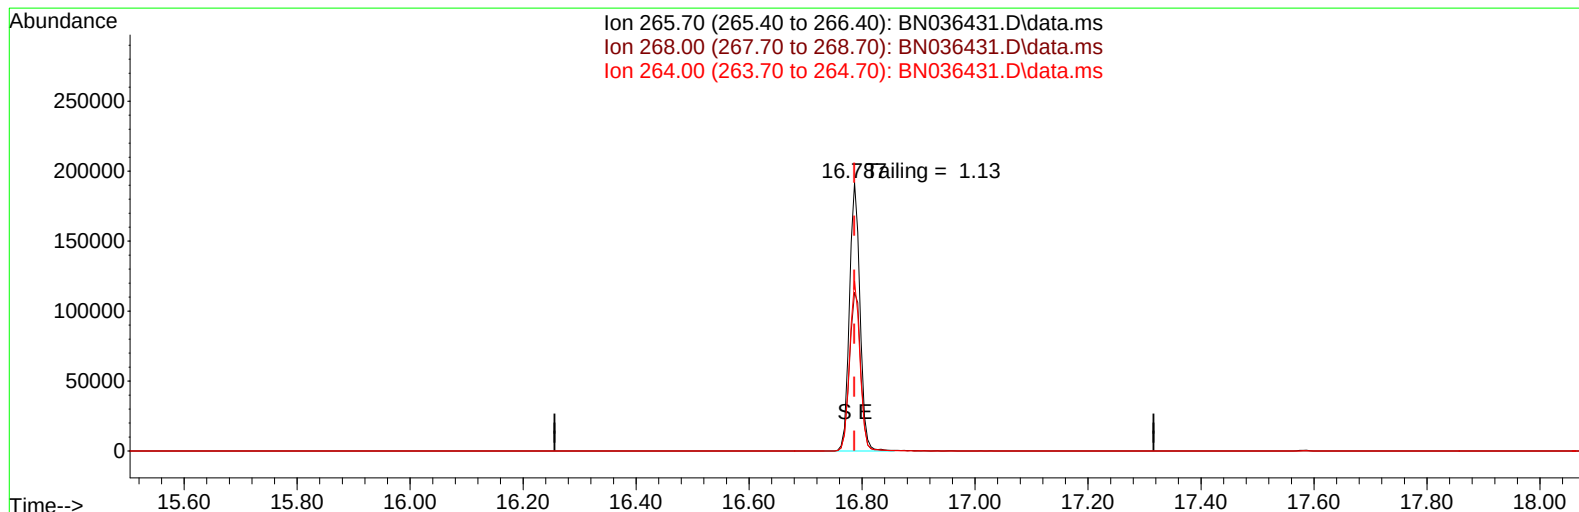

TIC: BN036431.D\data.ms

(70) Pentachlorophenol (C)




16.787min (+ 0.001) 19373.02 ng

response 250165

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.05
264.00	61.60	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021225\
Data File : BN036431.D
Acq On : 12 Feb 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 14:50:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 14:47:47 2025
Response via : Initial Calibration

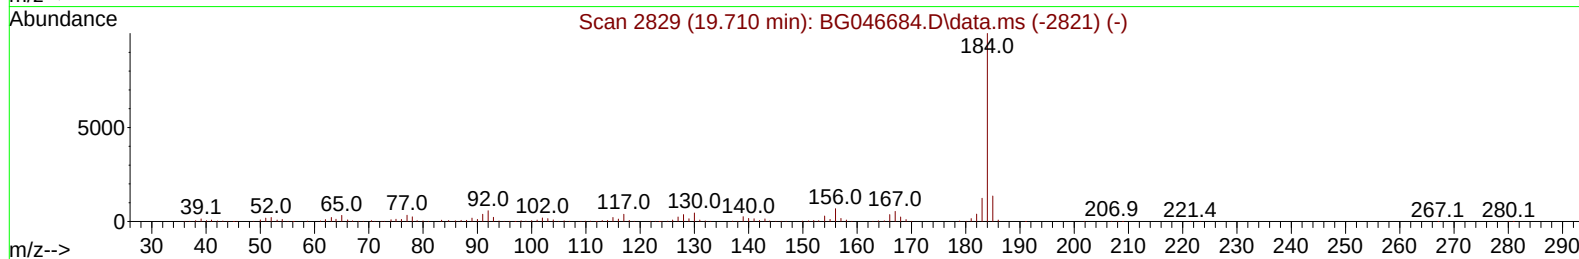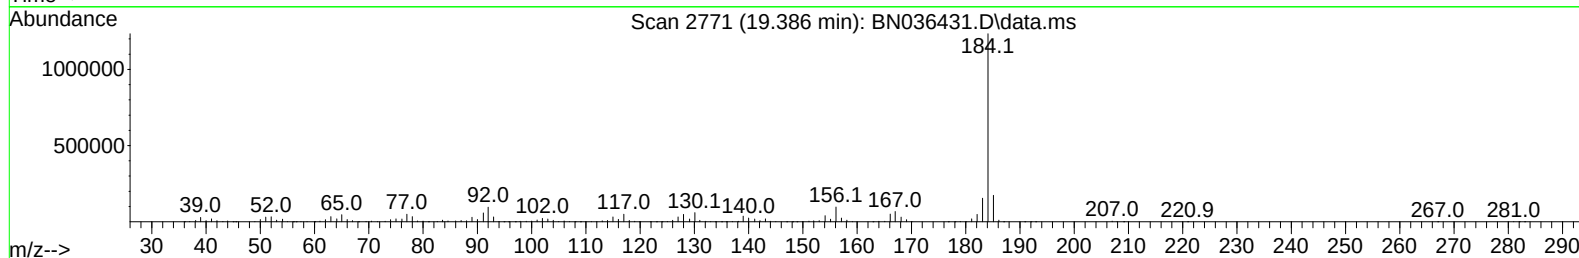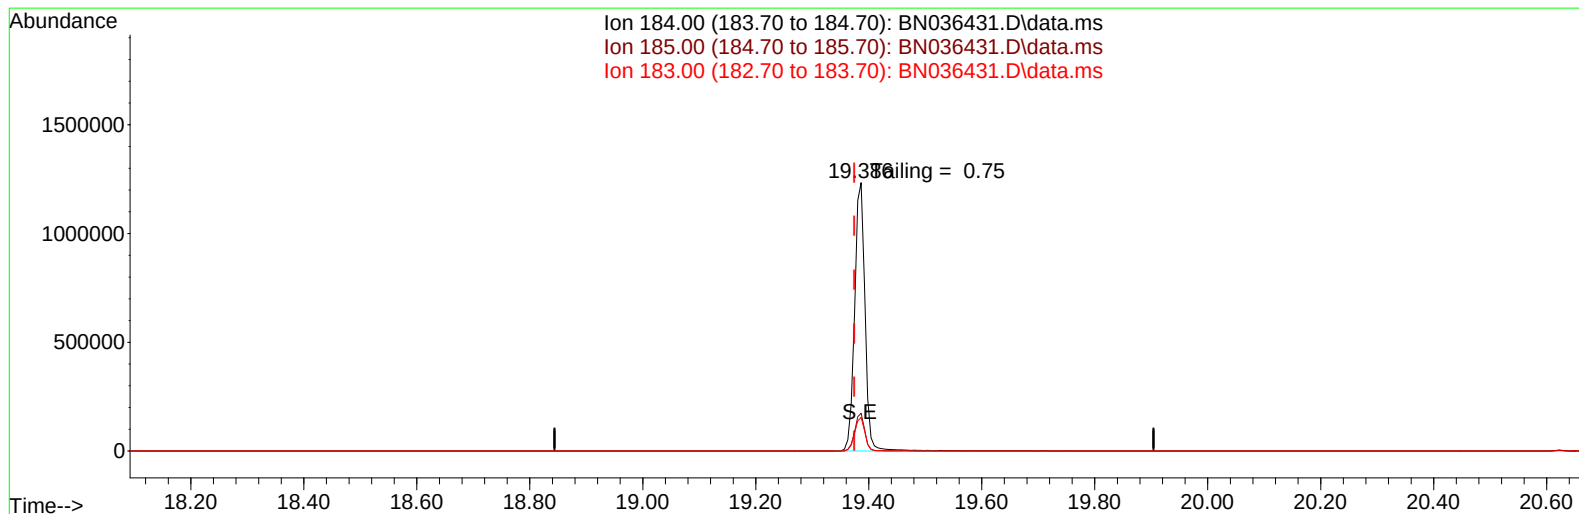

TIC: BN036431.D\data.ms

(77) Benzidine**19.386min (+ 0.012) 0.00 ng****response 1586765**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.08
183.00	13.20	12.56
0.00	0.00	0.00