
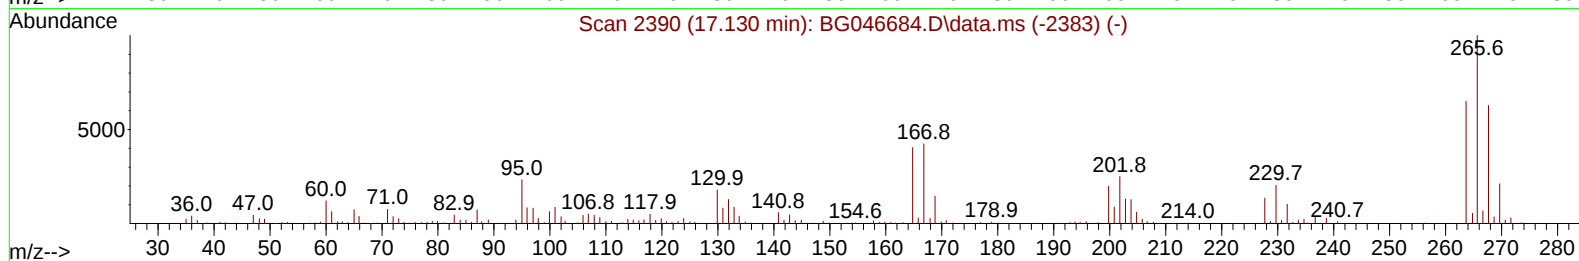
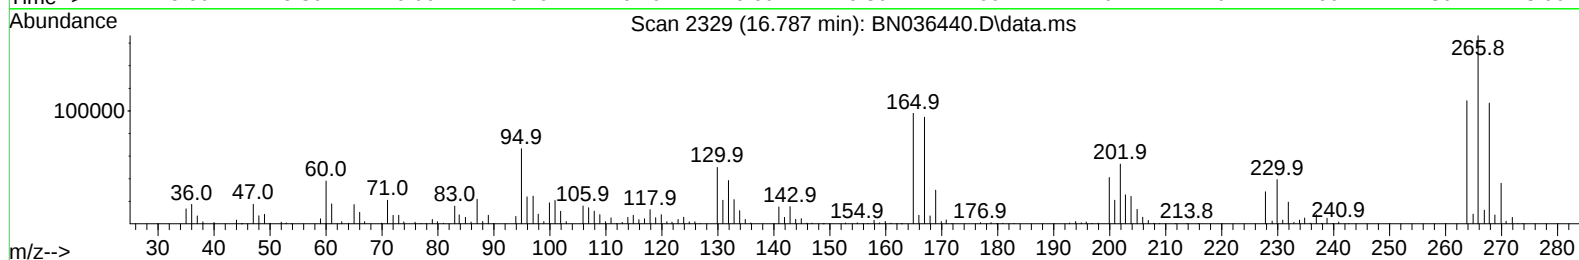


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021225\
Data File : BN036440.D
Acq On : 12 Feb 2025 15:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 17:06:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

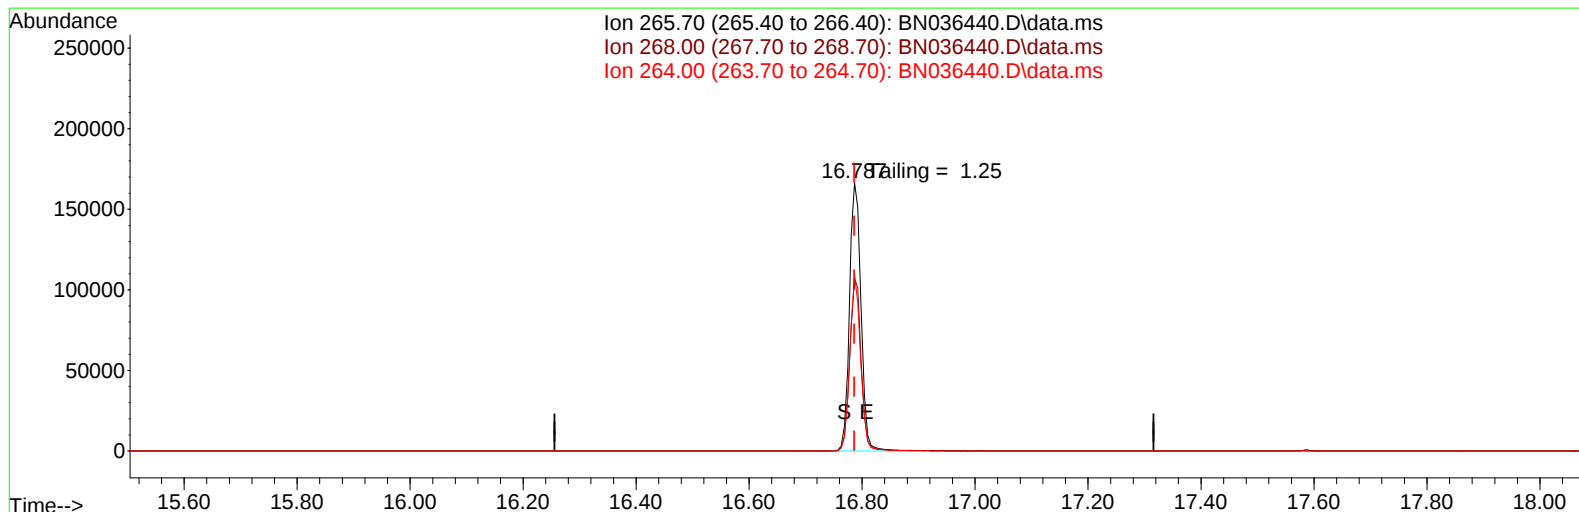

TIC: BN036440.D\data.ms

(70) Pentachlorophenol (C)




16.787min (+ 0.001) 20072.93 ng

response 236291

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.22
264.00	61.60	65.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021225\
Data File : BN036440.D
Acq On : 12 Feb 2025 15:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 17:06:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

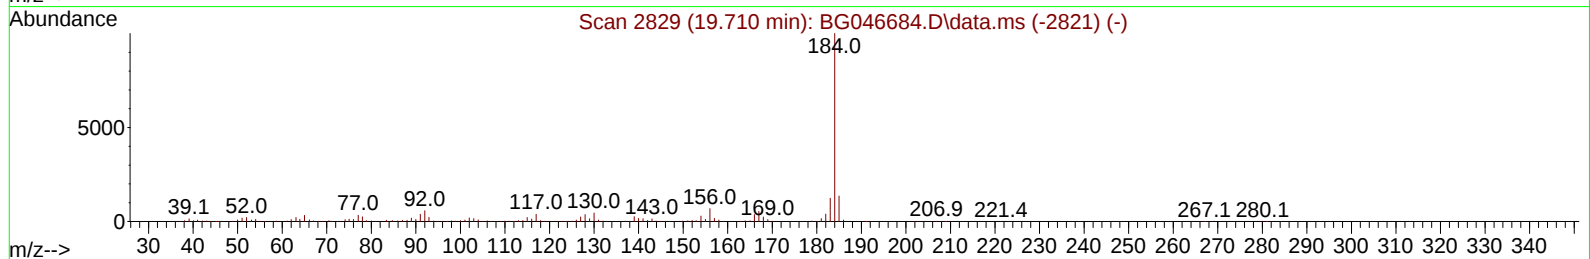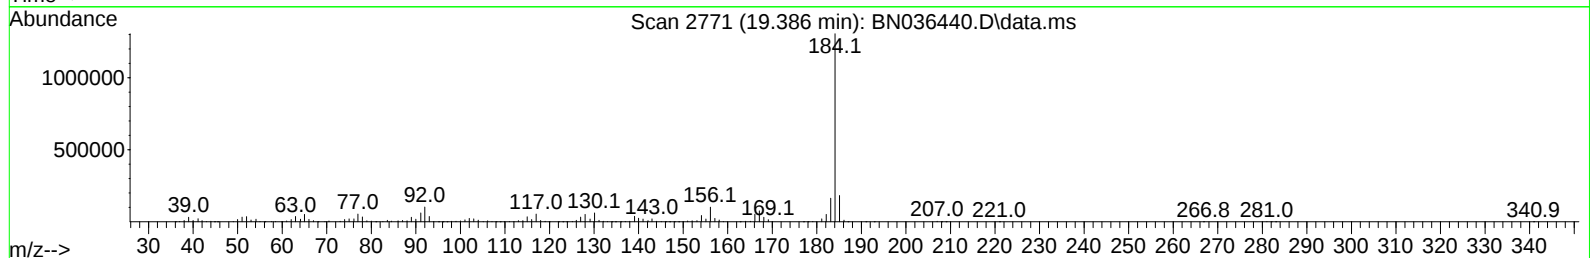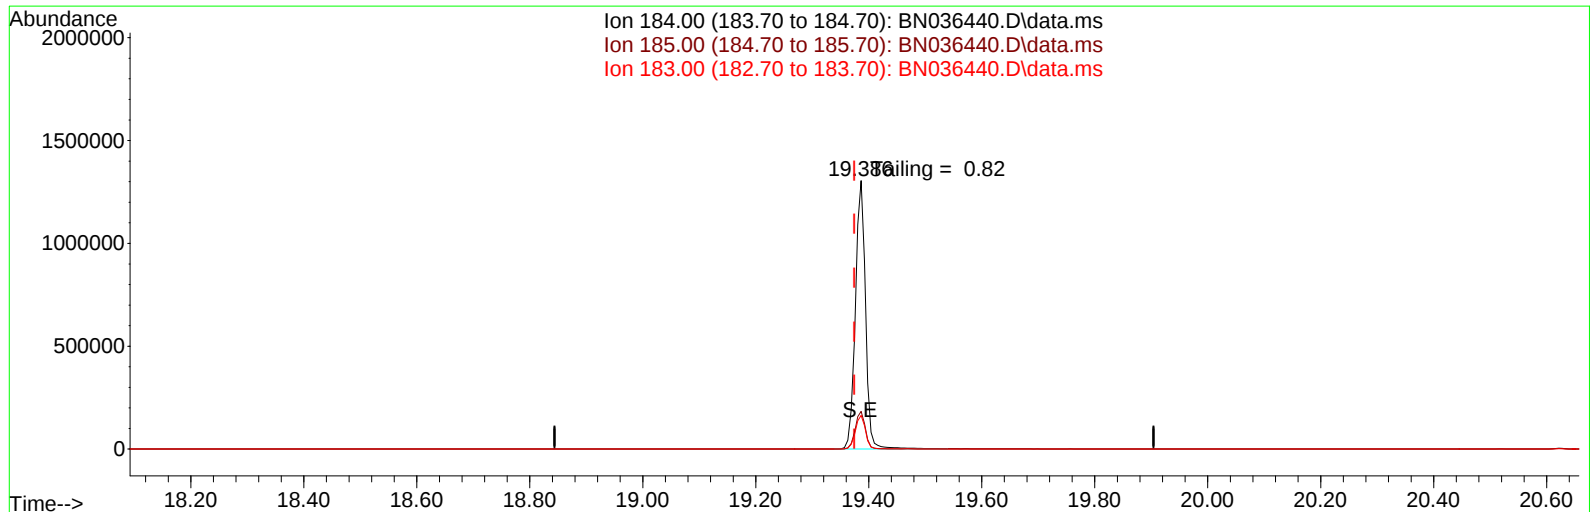

TIC: BN036440.D\data.ms

(77) Benzidine

19.386min (+ 0.012) 0.00 ng

response 1640537

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.01
183.00	13.20	12.53
0.00	0.00	0.00