
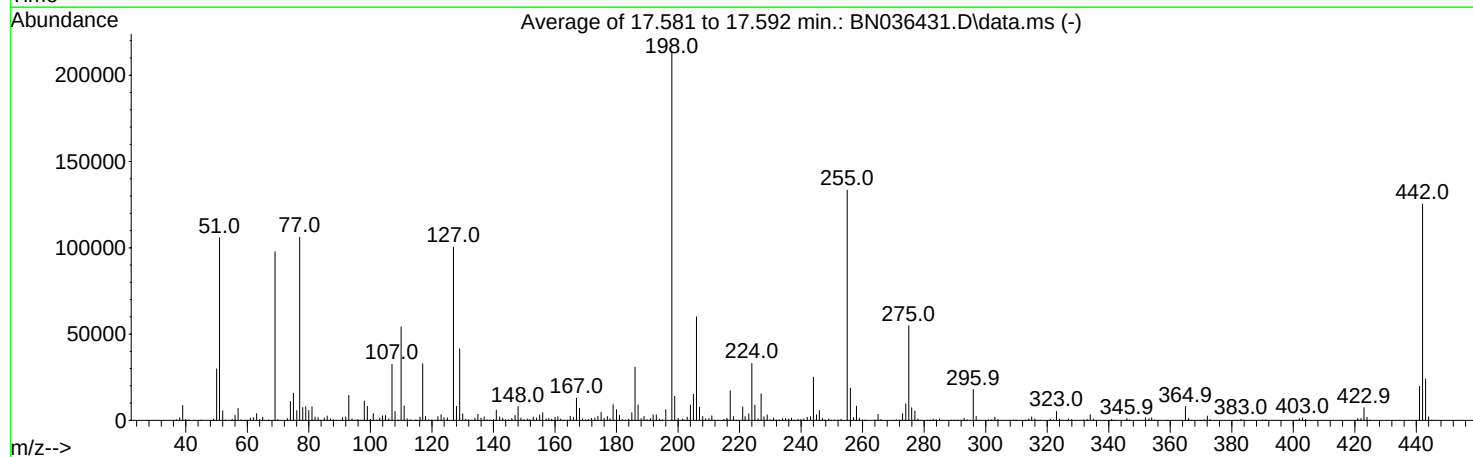


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021225\
Data File : BN036431.D
Acq On : 12 Feb 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 11 01:17:14 2025

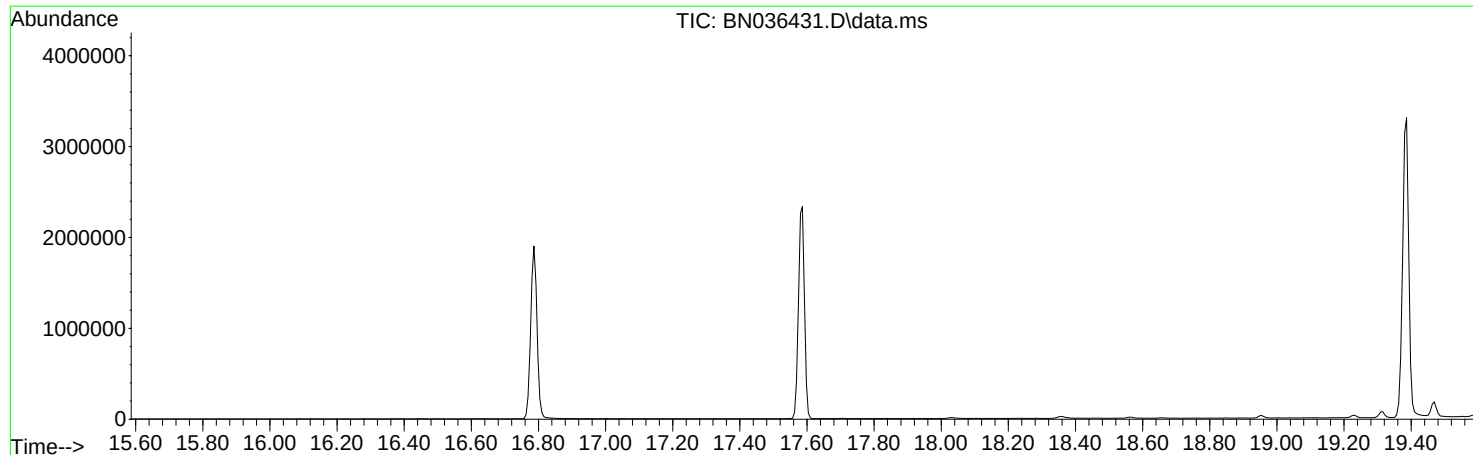

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.7	105897	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.8	97744	PASS
70	69	0.00	2	0.5	500	PASS
127	198	10	80	47.1	100381	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	213184	PASS
199	198	5	9	6.6	14015	PASS
275	198	10	60	25.7	54781	PASS
365	198	1	100	3.8	8019	PASS
441	198	0.01	100	9.2	19709	PASS
442	442	50	100	100.0	125331	PASS
443	442	15	24	19.1	23907	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/12/2025	BNA_N	<u>BN036431.D</u>
Compound Name	Response	Retention Time
DDT	837848	20.622
DDD	7901	20.233
DDE	0	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7901	845749	0.93

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021225\
Data File : BN036431.D
Acq On : 12 Feb 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 12 14:50:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 14:47:47 2025
Response via : Initial Calibration

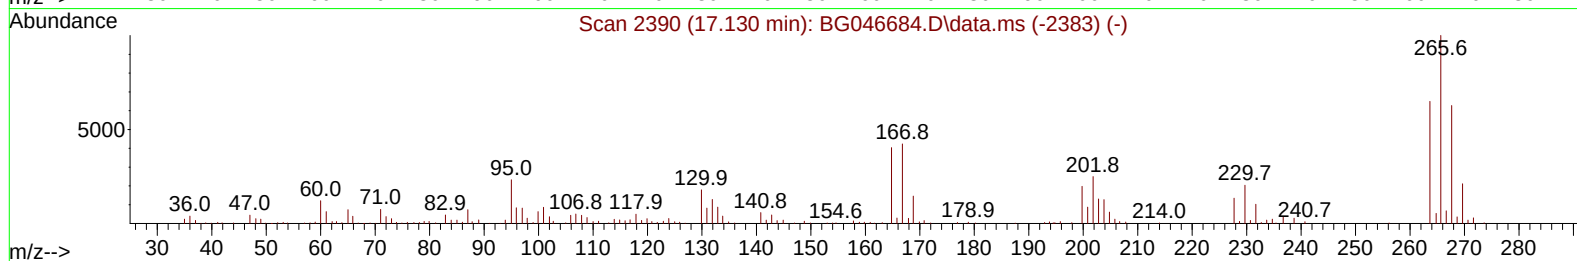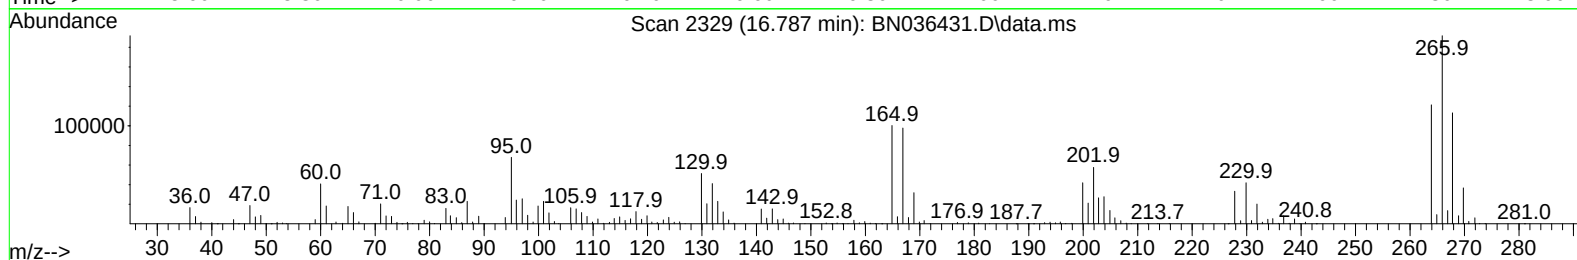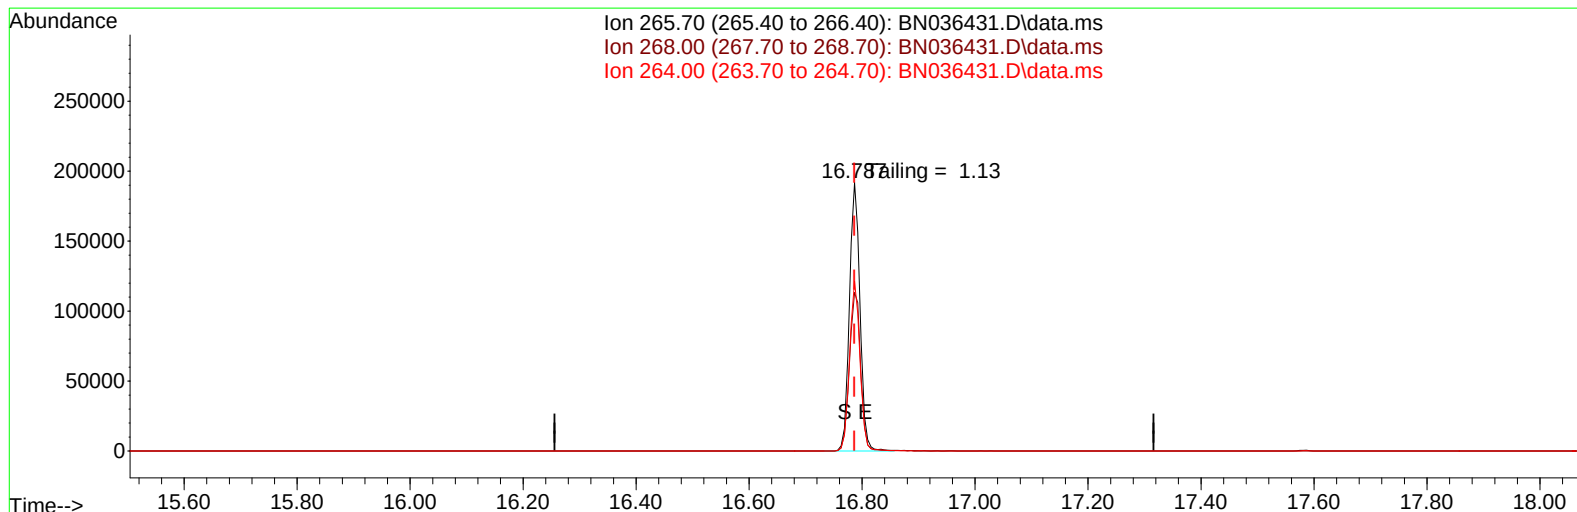

TIC: BN036431.D\data.ms

(70) Pentachlorophenol (C)

16.787min (+ 0.001) 19373.02 ng




response 250165

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.05
264.00	61.60	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021225\
Data File : BN036431.D
Acq On : 12 Feb 2025 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 12 14:50:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 12 14:47:47 2025
Response via : Initial Calibration

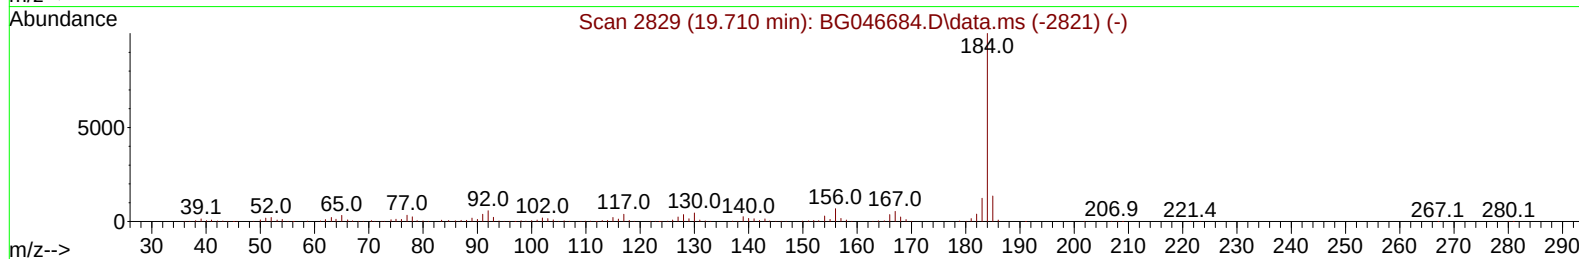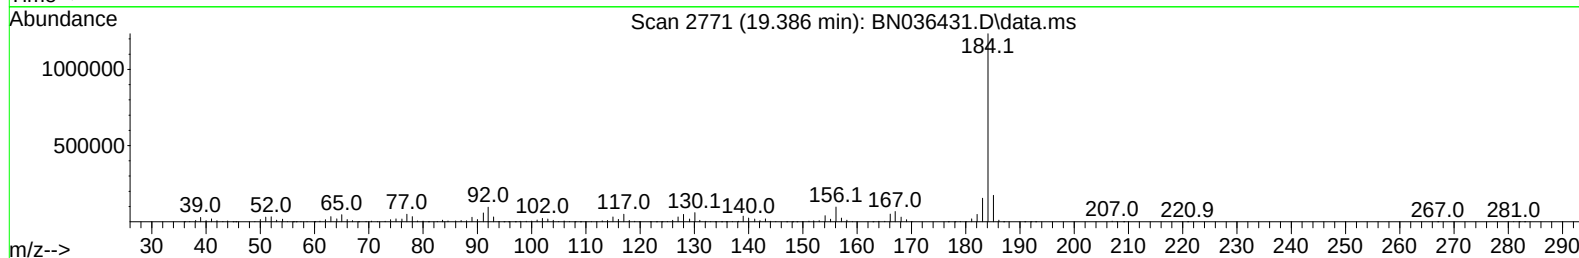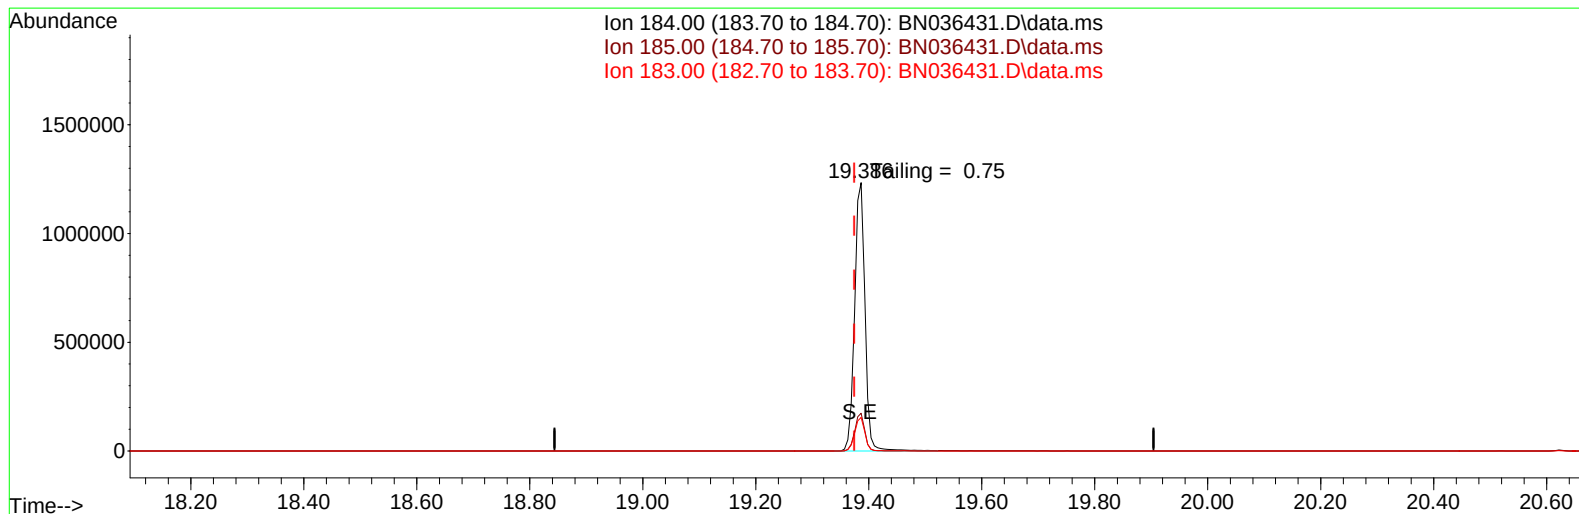

TIC: BN036431.D\data.ms

(77) Benzidine

19.386min (+ 0.012) 0.00 ng

response 1586765

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.08
183.00	13.20	12.56
0.00	0.00	0.00